

OSSTEM IMPLANT SYSTEM


2012 PRODUCT CATALOG



for **TS IMPLANT SYSTEM**

| | | | | |
|---|---|--|---|--|
| TS & GS System  |  20 TSII Fixture |  22 TSIII Fixture |  24 TSIII Ultra-Wide® Fixture |  26 TSIV Fixture |
|  28 GSII RBM Fixture |  30 GSII RBM Ultra-Wide® Fixture |  32 GSIII RBM Fixture |  34 Simple Mount |  34 Cover Screw |
|  35 Healing Abutment |  39 Rigid Abutment |  41 Rigid Protect Cap |  41 Rigid Impression Coping |  42 Rigid Burn-out cylinder |
|  42 Rigid Lab Analog |  43 Transfer Abutment |  43 Lab Screw |  43 Waxing Screw |  43 Fixture Lab Analog |
|  44 Bite Index |  44 Fixture Pick-up Impression Coping |  45 Fixture Transfer Impression Coping |  45 Temporary Abutment |  46 Angled Abutment |
|  46 GS Angled Abutment Selector |  47 ZioCera Abutment |  48 ZioCera Angled Abutment |  49 GoldCast Abutment |  50 NP-CAST Abutment |
|  51 CustomFit Abutment |  52 FreeForm ST Abutment |  53 Convertible Abutment |  53 Combination Cylinder |  53 Convertible Angled Cylinder |
|  54 Convertible GoldCast Cylinder |  54 Convertible Temporary Cylinder |  54 Convertible Plastic Cylinder |  55 Convertible Pick-up Impression Coping |  55 Convertible Transfer Impression Coping |
|  56 Convertible Protect Cap |  56 Convertible Lab Analog |  56 Convertible Polishing Protector |  57 Stud Abutment |  57 Stud Abutment Set (Dalbo Set) |

OSSTEM HISTORY

| | | | | |
|---|--|--|--|--|
|  58 O-ring Retainer Cap Set |  58 O-ring Retainer Set |  58 O-ring Set |  59 O-ring Lab Analog |  60 LOCATOR® Abutment |
|  60 LOCATOR® Male Processing Kit |  60 LOCATOR® Replacement Male |  61 LOCATOR® Extended Replacement Male |  61 LOCATOR® Black Processing Male |  61 LOCATOR® Block out Spacer |
|  61 LOCATOR® Impression Coping |  61 LOCATOR® Lab Analog |  62 LOCATOR® Core Tool |  62 LOCATOR® Torque Driver | |
| | | | | |
| | | | | |
| | | | | |
| | | | | |
| | | | | |
| | | | | |
| | | | | |
| | | | | |

| | | | | | | | | | | |
|------|------|---|--|---|---|---|--|---|---|---|
| 2011 | Dec | Introduces and commences commercial production of K2 Unit & Chair | 2007 | Mar | Develops and begins commercial production of MS Lists on KOSDAQ (KRX: Korea Exchange) | | | | | |
| | Nov | Develops and begins commercial production of Smart Membrane | | 2006 | Dec | Establishes subsidiary offices in Bangkok, Thailand and Kuala Lumpur, Malaysia [OSSTEM Thailand Co., Ltd. and OSSTEM Malaysia SDN, BHD] | | | | |
| | Oct | Registers and obtains approval from Health Canada Develops and begins commercial production of USII SA and 123 Kit | | | Nov | Registers and obtains approval from the SFDA in China | | | | |
| | Sep | Establishes subsidiary offices in Dacca , Bangladesh and Ho Chi Minh City, Vietnam [OSSTEM Bangladesh Ltd. and OSSTEM IMPLANT Vina Co., Ltd.] Develops and begins commercial production of SSIII SA Registers and obtains approval from the Ministry of Health and Society in Vietnam | | | Sep | Establishes subsidiary office in Philadelphia, U.S.A [HiOssen Inc.] | | | | |
| | Aug | Establishes subsidiary offices in Manila, Philippines and Vancouver, Canada [OSSTEM Philippines Inc. and HiOssen Implant Canada Inc.] | | | Aug | Establishes subsidiary offices in Beijing, China / Singapore and Hong Kong [OSSTEM China Co., Ltd. / OSSTEM Singapore Pte Ltd. and OSSTEM Hong Kong Ltd.] | | | | |
| | Jul | Develops and begins commercial production of CustomFit Abutment Establishes subsidiary offices in Almaty, Kazakhstan [OSSTEM IMPLANT LLP] | | | Jul | Establishes subsidiary office in Tokyo, Japan [OSSTEM Japan Corp.] | | | | |
| | Jun | Develops and begins commercial production of TSII SA Hosts 'OSSTEM World Meeting 2011 in Seoul' | | | Apr | Registers and obtains the GOST-R certification in Russia Opens 'OSSTEM World Meeting 2006 in Seoul' Publishes the '2006 OSSTEM IMPLANT SYSTEM' - Introduction and particulars of implant system | | | | |
| | Apr | Develops and begins commercial production of LAS Kit Establishes subsidiary offices in Jakarta, Indonesia [PT OSSTEM Indonesia] | | | Jan | Establishes the subsidiary offices in Moscow, Russia and Mumbai, India [OSSTEM LLC. and OSSTEM IMPLANT India Pvt Ltd.] | | | | |
| | Mar | Establishes subsidiary offices in Guadalajara, Mexico [HiOssen de Mexico] | | | 2005 | Dec | Registers and obtains approval by the DOH in Taiwan Establishes the subsidiary office in Ashborn, Germany [OSSTEM Germany GmbH] | | | |
| | Feb | Develops and begins commercial production of TSIV SA | | | | May | Develops and begins commercial production of GSII | | | |
| 2010 | Nov | Develops and begins commercial productions of SSII SA | Apr | | | Hosts 'OSSTEM World Meeting 2005 in Seoul' | | | | |
| | Aug | Develops and begins commercial productions of TSIII Ultra-wide | Mar | Obtains KGMP(Korean Good Manufacturing Practice) in Korea | | | | | | |
| | Jun | Develops and begins commercial productions of TSIII HA and CAS Kit Opens 'OSSTEM World Meeting 2010 in Beijing' | Jan | Establishes the subsidiary office in Taipei, Taiwan [OSSTEM Corporation] | | | | | | |
| | Apr | Develops and begins commercial productions of Osstem Guide | 2004 | Nov | | Develops and begins commercial production of SSIII | | | | |
| | Mar | Develops and begins commercial productions of TSIII SA | | Jul | | Develops and begins commercial production of USIII | | | | |
| | 2009 | Oct | | Registers and obtains approval from Health, Labor and Welfare in Japan | | Apr | Opens 'OSSTEM World Meeting 2004 in Seoul' | | | |
| | | May | | Hosts 'OSSTEM World Meeting 2009 in Bangkok' | | 2002 | Oct | Develops and begins commercial production of SSII | | |
| | | Jan | | Certifies PEP7 (the world's first new Osseo-inductive compound) | | | Aug | Registers and obtains approval by the FDA in the USA Develops and begins commercial production of USII | | |
| | | 2008 | | Nov | Develops and begins commercial productions of SS Ultra-wide | | Jan | Establishes OSSTEM Implant R&D Center | | |
| | | | | Jun | Develops and begins commercial productions of GSIII | | 2001 | Mar | Establishes AIC(Apsun Dental Implant Research & Education Center) | |
| Apr | | | | Hosts 'OSSTEM World Meeting 2008 in Seoul' | Jan | | | Obtains CE-0434 certification | | |
| Mar | | | | Opens ATC Training Center | 1999 | | | Dec | Obtains ISO-9001 certification | |
| Jan | | | | Establishes OSSTEM Bone Science Institute | | | | 1997 | Dec | Begins commercial production under the brand name of OSSTEM |
| 2007 | | | Oct | Establishes subsidiary offices in Sydney, Australia [Osstem Australia PTY Ltd.] | | | | | Jan | Establishes OSSTEM IMPLANT Co., Ltd. in Seoul, Korea |
| | | | Jun | Registers and obtains approval from the TGA in Australia | | | | | 1995 | |
| | May | | Develops and begins commercial production of US Ultra-wide | 1992 | | | | | | |
| | Apr | | Hosts 'OSSTEM World Meeting 2007 in Seoul' Begins commercial production of V-ceph | | | | | | | |

CHARACTERISTIC of OSSTEM IMPLANT SYSTEM

OSSTEM Implant key reference (as of Mar.2012)

■ TS/GS System - Clinic

| No. | Title | Reference | Author |
|-----|---|---|-----------------------|
| 1 | Comparison of Clinical Outcomes of Sinus Bone Graft with Simultaneous Implant Placement: 4-month and 6-month Final Prosthetic Loading | Oral Surg Oral Med Oral Pathol Oral Radiol Endod. 2011 Feb;111(2):164-9 | Young-Kyun Kim et al. |
| 2 | Prospective study of tapered RBM surface implant stability in the maxillary posterior area | Accepted in 2011 Oral Surg Oral Med Oral Pathol Oral Radiol Endod. | Young-Kyun Kim et al. |
| 3 | A 1-year Prospective Clinical Study of Soft Tissue Conditions and Marginal Bone Changes around Dental Implants after Flapless Implant Surgery | Oral Surg Oral Med Oral Pathol Oral Radiol Endod. 2011 Jan;111(1):41-6 | Seung-Mi Jeong et al. |
| 4 | Short-Term Retrospective Clinical Study of Resorbable Blasting Media Surface Tapered Implants. | J Korean Assoc Maxillofac Plast Reconstr Surg 2011;33(2):149-53 | Young-Kyun Kim et al. |
| 5 | Early loading after sinus bone graft and simultaneous implant placement | Australasian Dental Practice 2011(March/April): 136-42 | Young-Kyun Kim et al. |
| 6 | Evaluation of the feasibility of bony window repositioning without using a barrier membrane in sinus lateral approach | J Korean Assoc Oral Maxillofac Surg 2011;37(2):122-6 | Chang-Joo Park et al. |
| 7 | A short-term clinical study of marginal bone level change around microthreaded and platform-switched implants | J Periodontal Implant Sci 2011;41:211-7 | Kyoo-Sung Cho et al. |
| 8 | Analysis of Prognostic Factors after a Variety of Osstem® Implant Installation | J Korean Implantology(KAOMI) 2011;15(2):170-9 | Young-Kyun Kim et al. |
| 9 | Clinical Comparison of Immediately Loaded and Delayed Loaded OSSTEM GSIII Implant in Partially Edentulous Patients | J Kor Stomatognathic Function occlusion 2011;27(3):267-75 | Yang-Jin Yi et al. |
| 10 | A Prospective Multicenter Study on the Clinical Success Rate of the Osstem Implant (New GSII RBM) in Edentulous Patients | J Korean Implantology(KAOMI) 2011;15(2):142-52 | Su-Kwan Kim et al. |
| 11 | A Relaxed Implant Bed: Implants Placed After Two Weeks of Osteotomy with Immediate Loading - A One Year Clinical Trial | Accepted in 2010 for Publication in J Oral Implantol. | Bansal DJ et al. |
| 12 | Subjective satisfaction of clinician and Short-term Clinical Evaluation of Osstem TSIII SA Implant | J Korean Clinical Implant 2010;30(7):430-43. | Young-Kyun Kim et al. |
| 13 | Short-term, Multi-center Prospective Clinical Study of Short Implants Measuring Less than 7mm | J Kor Dent Sci 2010;3(1):11-6 | Young-Kyun Kim et al. |
| 14 | Effects of Flapless Implant Surgery on Soft Tissue Profiles: A Prospective Clinical Study | Clin Implant Dent Relat Res. 2011 Dec;13(4):324-9 | Byung-Ho Choi et al. |
| 15 | Evaluation of Survival Rate and Crestal Bone Loss of the Osstem GS II Implant System | J Kor Dent Sci. 2009;3(1):30-3 | Young-Kyun Kim et al. |
| 16 | Analysis of factors affecting crestal bone loss around the implants | J Kor Dent Sci. 2009;3(1):12-7 | Young-Kyun Kim et al. |
| 17 | Retrospective study of GS II Implant(Osstem) with an internal connection with microthreads | J Kor Stomatognathic Function occlusion 2009;25(4):417-29 | Young - Deok, Chee |
| 18 | Study On Radiographic Evaluation of Marginal Bone Loss Around Osseointegrated Implant after Functional Loading | J Kor Oral Maxillofac Surg 2009;35:240-7 | Se-Wook Koh et al. |
| 19 | Evaluation of Sinus Bone Resorption and Marginal Bone Loss after Sinus Bone Grafting and Implant Placement | Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2009;107:e21-8 | Young-Kyun Kim et al. |
| 20 | Evaluation of Periimplant Tissue Response according to the Presence of Keratinized Mucosa | Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2009;107:e24-8 | Young-Kyun Kim et al. |
| 21 | The Use of Buccinator Musculomucosal Flap in Implant | Accepted in 2009 for Publication in Int J Periodontics Restorative Dent | Young-Kyun Kim et al. |
| 22 | Observation of the Change of the Dental Implant Stability and Bone Density Evaluation Methods | J Korean Acad Periodontol 2009;39(2):185-92 | Sok-Min Ko et al. |
| 23 | Clinical and Radiographic Evaluation of Implants with Dualmicrothread: 1-year Study | J Korean Acad Periodontol 2009;39(1):27-36 | Ju-Youn Lee et al. |
| 24 | Short term Retrospective Clinical Study on GS II, SS III, US III | J Korean Implantology(KAOMI) 2008;12(2):12-22 | Young-Kyun Kim et al. |
| 25 | Analysis of Clinical Application of Osstem (Korea) Implant System for 6 Years | J Korean Implantology(KAOMI) 2006;10(1):56-65 | Young-Kyun Kim et al. |

■ TS/GS System - Biology

| No. | Title | Reference | Author |
|-----|--|---|------------------------|
| 1 | Effects of Soft Tissue Punch Size on the Healing of Peri-implant Tissue in Flapless Implant Surgery. | Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2010;109:525-30. | Byung-Ho Choi et al. |
| 2 | The Use of Autologous Venous Blood for Maxillary Sinus Floor Augmentation in Conjunction with Sinus Membrane Elevation: An Experimental Study. | Clin. Oral Impl. Res. 2010;21:346-9. | Byung-Ho Choi et al. |
| 3 | Morphogenesis of the Peri-Implant Mucosa: A Comparison between Flap and Flapless Procedures in the Canine Mandible | Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2009;107:66-70 | Byung-Ho Choi et al. |
| 4 | Blood Vessels of the Peri-Implant Mucosa: A Comparison between Flap and Flapless Procedures | Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2009;107:508-12 | Byung-Ho Choi et al. |
| 5 | Simultaneous Flapless Implant Placement and Peri-Implant Defect Correction: An Experimental Pilot Study in Dogs | J Periodontol 2008;79:876-80 | Byung-Ho Choi et al. |
| 6 | The Effect of Thick Mucosa on Peri-implant Tissues: An Experimental Study in Dogs | J Periodontol 2008;79(11):2151-5 | Byung-Ho Choi et al. |
| 7 | Er:YAG Laser Irradiated Implant Surface Observation with Scanning Electron Microscopy | J Korean Assoc Maxillofac Plast Reconstr Surg 2008;30(6):540-5 | Seung-Ki Min et al. |
| 8 | Comparative Study of Removal Effect on Artificial Plaque from RBM Treated Implant | J Korean Assoc Maxillofac Plast Reconstr Surg 2007;29(4):309-20 | Hee-Jyun Oh et al. |
| 9 | The Effect of Ca-P Coated Bovine Mineral on Bone Regeneration around Dental Implant in Dogs | J Korean Acad Periodontol 2006;36(4):913-23 | Seoung-Ho Lee et al. |
| 10 | Scanning Electron Microscopic Study of Implant Surface after Er,Cr:YSGG Laser Irradiation | J Korean Assoc Maxillofac Plast Reconstr Surg 2006;28(5):454-69 | Kyung-Hwan Kwon et al. |

■ TS/GS System - Biomechanics

| No. | Title | Reference | Author |
|-----|--|--|------------------------|
| 1 | Variation in the Total Lengths of Abutment/Implant Assemblies Generated with a Function of Applied Tightening Torque in External and Internal Implant-Abutment Connection. | Clin. Oral Impl. Res. 2011;22:834-9. | Ki-Seong Kim et al. |
| 2 | self-cutting blades and their influence on primary stability of tapered dental implants in a simulated low-density bone model: a laboratory study | Pathol. Oral. Radiol. Endod. 2011;112:573-580 | Young-Jun Lim et al. |
| 3 | Screw Joint Stability under Cyclic Loading of Zirconia Implant Abutments | J Kor Acad Prosthodont 2009;47(2):164-73 | Jae-Jun Ryu et al. |
| 4 | Fatigue Characteristics of Five Types of Implant-Abutment Joint Designs | METAL AND MATERIALS International 2008;14(2):133-8 | Chang-Mo Jeong et al. |
| 5 | Influence of Tightening Torque on Implant-Abutment Screw Joint Stability | J Kor Acad Prosthodont 2008;46(4):396-408 | Chang-Mo Jeong et al. |
| 6 | Effect of Casting Procedure on Screw Loosening of UCLA Abutment in Two Implant-Abutment Connection Systems | J Kor Acad Prosthodont 2008;46(3):246-54 | Myung-Joo Kim et al. |
| 7 | Evaluation of Stability of Double Threaded Implant-Emphasis on Initial Stability Using Osstell Mentor™; Part I | J Kor Acad Stomatog Func Occlusion 2007;23(4) | Yong-Deok Kim et al. |
| 8 | Influence of Tungsten Carbide/Carbon Coating of Implant-Abutment Screw on Screw Loosening | J Kor Acad Prosthodont 2008;46(2):137-47 | Chang-Mo Jeong et al. |
| 9 | The Assessment of Abutment Screw Stability Between the External and Internal Hexagonal Joint under Cyclic Loading | J Kor Acad Prosthodont 2008;46(6):561-8 | Jung-Suk Han et al. |
| 10 | Influence of Implant Fixture Design on Implant Primary Stability | J Kor Acad Prosthodont 2006;45(1):98-106 | Seok-Gyu Kim et al. |
| 11 | Detorque Force of TiN-Coated Abutment Screw with Various Coating Thickness after Repeated Closing and Opening. | J Kor Acad Prosthodont 2007;45(6):769-79 | Chae-Heon Chung et al. |

OSSTEM Implant System Flow

| TSII | GSII RBM | TSIII | GSIII RBM |
|--|--|--|---|
| <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection Stable connection of the upper part based on Rigid Motion Connection SA surface morphology and roughness increased by 45% compared to RBM treatment Straight body facilitates the adjustment of implantation depth Powerful Self threading | <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection Harmonious macro & micro threads taking cortical bones and cancellous bones into consideration Expanded thread that helps have excellent initial stability Stable connection of the upper part based on Rigid Motion Connection RBM surface with excellent bio-affinity Straight body with the implant depth adjusted easily Implement the cutting edge with excellent self tapping capacity Realize the convenient operation by making it possible to implant into various osseins | <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection The initial stability for immediate & early loading The good feeling of fixture implantation The convenience of implant surgery Stable connection of the upper part based on Rigid Motion Connection SA surface morphology and roughness increased by 45% compared to RBM treatment Realize the convenient operation by making it possible to implant into various osseins | <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection The initial stability for immediate & early loading The good feeling of fixture implantation The convenience of implant surgery Stable connection of the upper part based on Rigid Motion Connection RBM surface with excellent bio-affinity Realize the convenient operation by making it possible to implant into various osseins |
| | | | |
| L: 8.5 10 11.5 13 15 | L: 8.5 10 11.5 13 15 | L: 8.5 10 11.5 13 15 | L: 8.5 10 11.5 13 15 |
| | | | |
| L: 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 15 |
| | | | |
| L: 6 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 15 | L: 6 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 15 |

| TSIII Ultra-Wide® | TSIV | GSII RBM Ultra-Wide® |
|---|---|--|
| <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection SA surface morphology and roughness increased by 45% compared to RBM treatment. Compatible with GS Regular abutment components Wide Diameter Fixture Indication <ul style="list-style-type: none"> Immediate placement at the extract socket Immediate replacement of the failed implant The actual length of TSIII Ultra-Wide Fixture is 0.5mm shorter than actual length. (Exception 7mm) | <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection SA surface morphology and roughness increased by 45% compared to RBM treatment. Specially developed for maxilla and soft bones <ul style="list-style-type: none"> High success rate even with poor bone quality. Improved design for initial stability and simplified surgical sequences <ul style="list-style-type: none"> Improved the initial stability with improved application of helical cutting, corkscrew thread, and sharp and rounded apex design | <ul style="list-style-type: none"> Bone level fixture of Internal Hex & 11° morse taper connection RBM surface with excellent bio-affinity Compatible with GS Regular abutment components Wide Diameter Fixture <ul style="list-style-type: none"> Indication <ul style="list-style-type: none"> Immediate placement at the extract socket Immediate replacement of the failed implant The actual length of GSII RBM Ultra-Wide Fixture is 0.5mm shorter than actual length. (Exception 7mm) |
| | | |
| L: 6 7 8.5 10 11.5 13 15 | L: 7 8.5 10 11.5 13 | L: 6 7 8.5 10 11.5 13 |

TS & GS Prosthesis Library



| Type | Abutment | Protect Cap | Retraction Cap | Impression coping |
|----------------------------|----------|-----------------------------|----------------|---------------------------|
| Rigid | | | | |
| Transfer | | | | |
| Angled | | | | |
| ZioCera/ ZioCera Angled | | | | |
| GoldCast/ NP-CAST | | | | |
| CustomFit | | | | |
| FreeForm ST | | | | |
| Convertible | | | | |
| Stud | | | | O-rings System |
| LOCATOR® | | Replacement Male | | |

| | Lab Analog | Burn-out Cylinder | Etc |
|---------------------|------------|---------------------------|------------------------------|
| | | | |
| | | Temporary Abutment | Bite Index |
| | | | |
| | | Cylinder | Polishing Protect Cap |
| | | | |
| Dalbo System | | | |
| | | Core Tool | Torque Driver |
| | | | |

TS & GS SYSTEM

TS & GS SYSTEM

OSSTEM IMPLANT SYSTEM

TS & GS System

Fixture and Restorative
Components




Early & Esthetic
OSSTEM IMPLANT

TS & GS System


Prosthetic Flow Diagrams for TS & GS System

Cement Retained Restoration : Rigid & Transfer Abutment • Mini, Regular

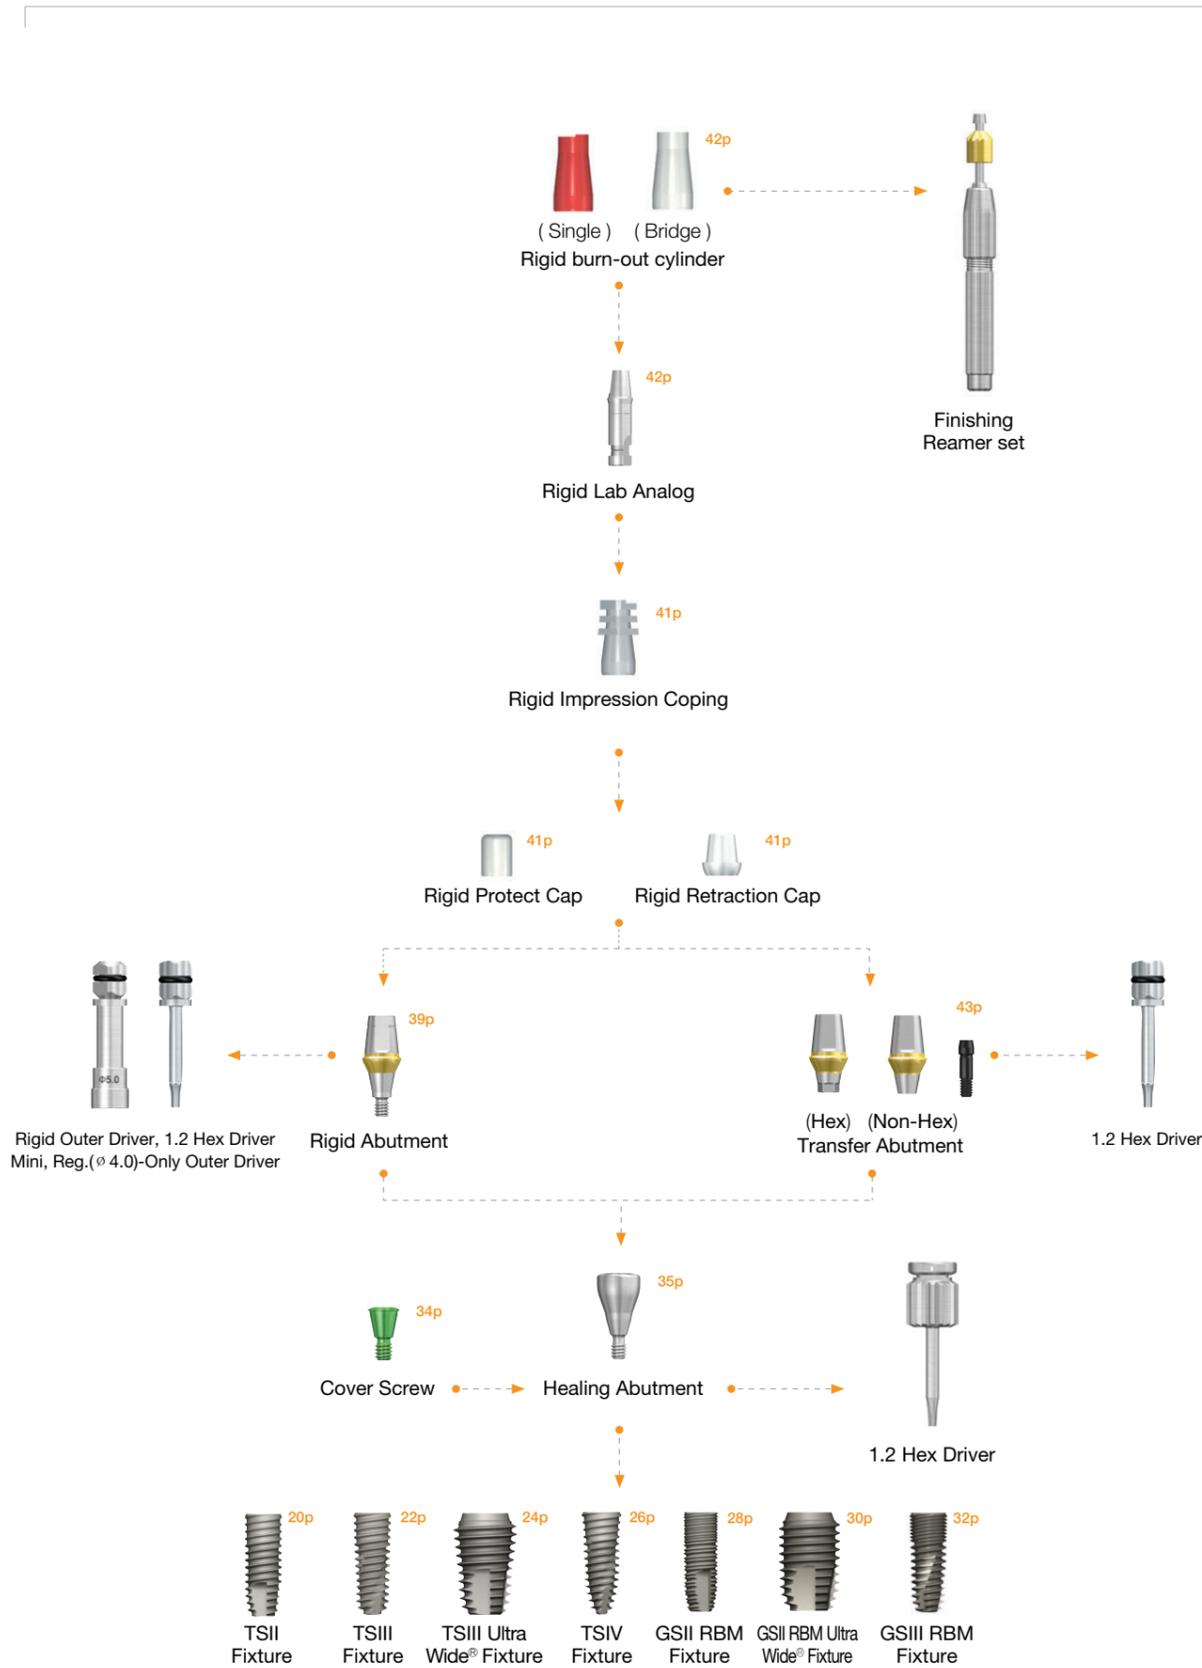


Prosthetic Flow Diagrams for TS & GS System

Cement Retained Restoration : Transfer, Angled, ZioCera, ZioCera Angled, GoldCast, CustomFit, NP-CAST, FreeForm ST
Screw Retained Restoration : ZioCera, ZioCera Angled, GoldCast, Temporary, NP-CAST Abutment • Mini, Regular

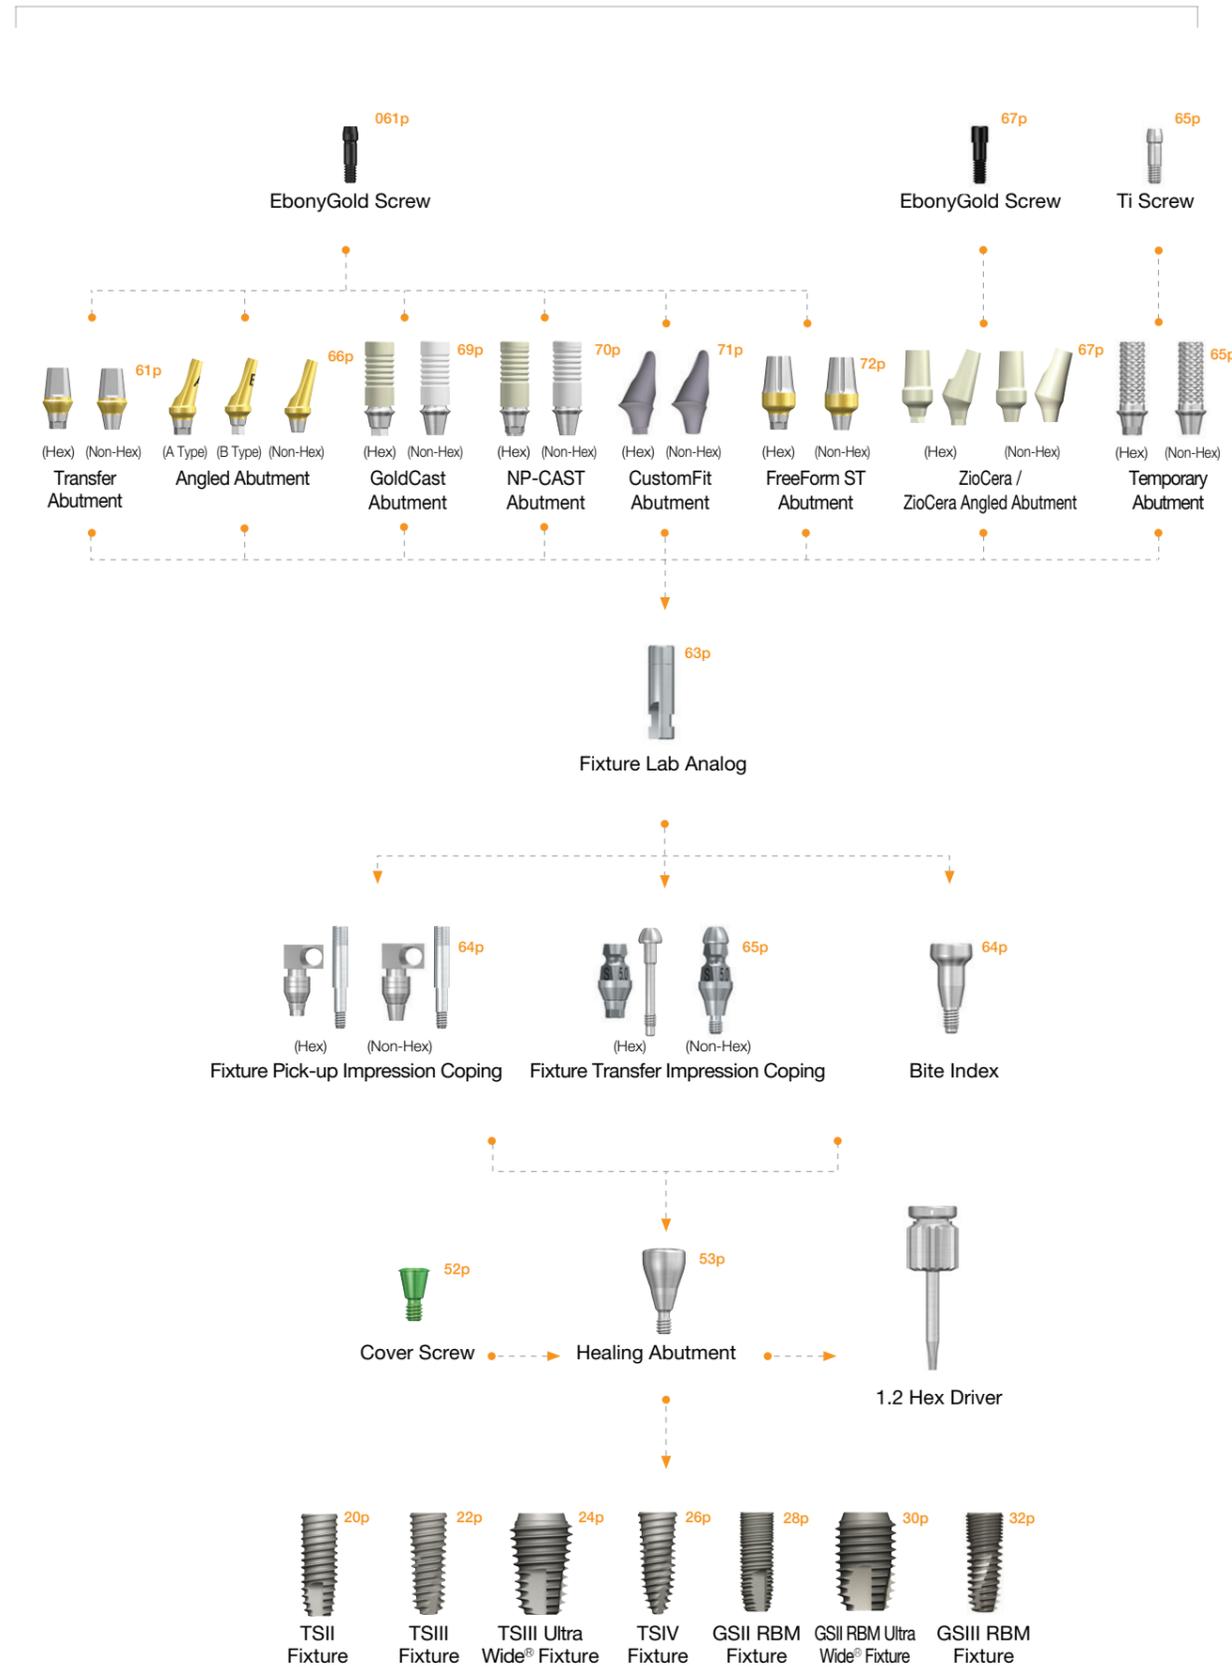


Prosthetic Flow Diagrams for TS & GS System

Screw & Cement Retained Restoration : Convertible Abutment • Mini, Regular

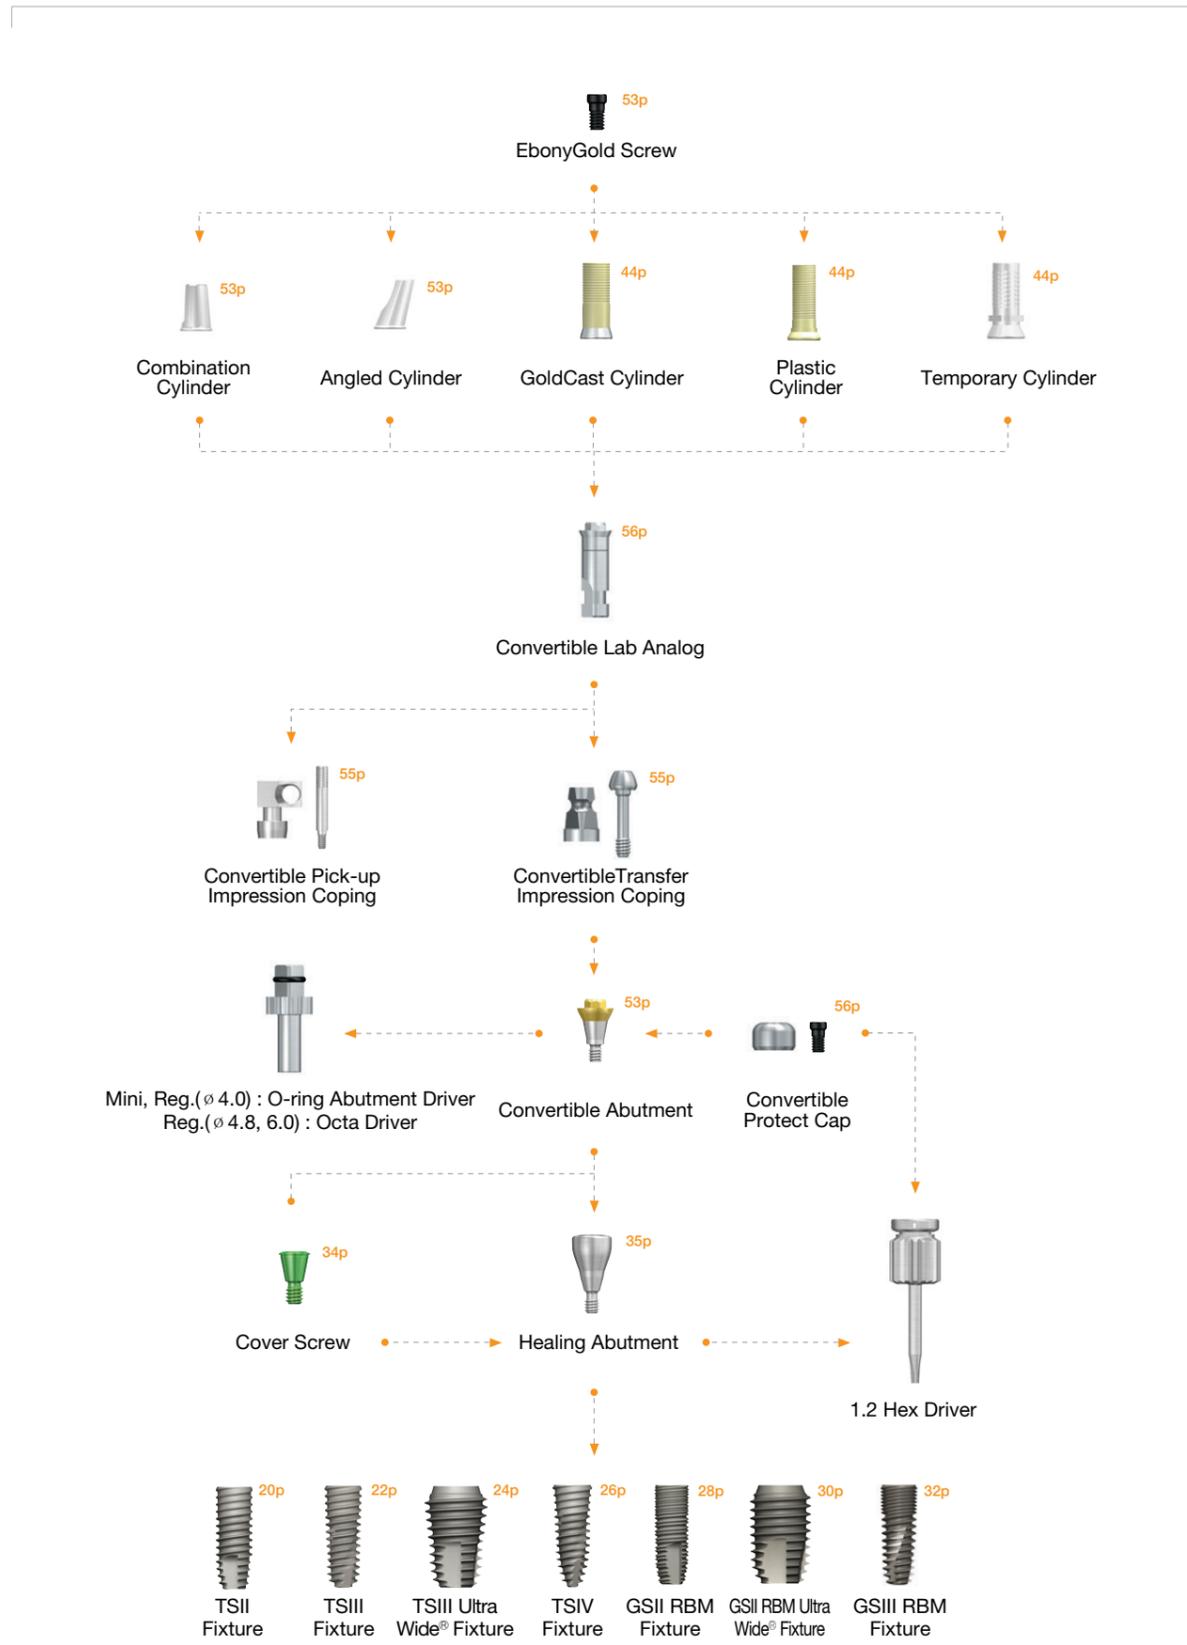


Prosthetic Flow Diagrams for TS & GS System

Overdenture Restoration : Stud / LOCATOR® Abutment • Mini, Regular

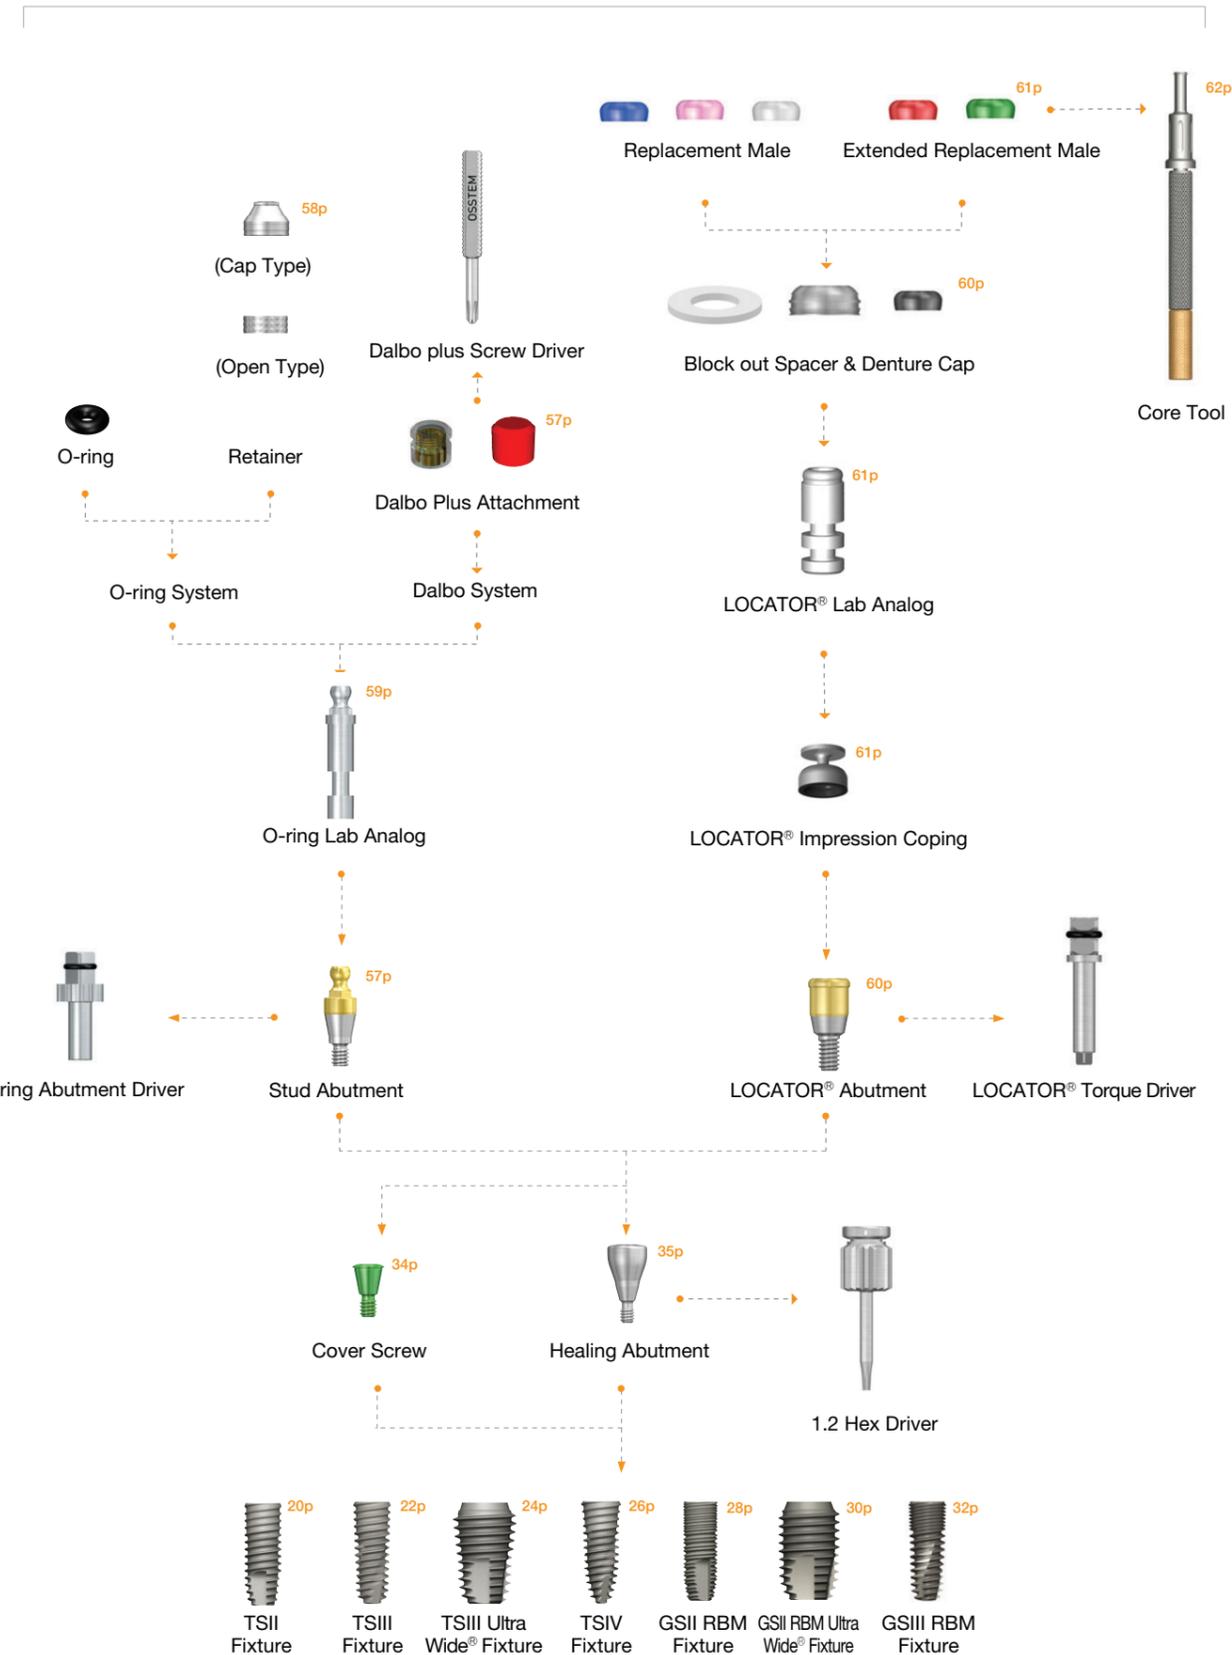

TSII Fixture

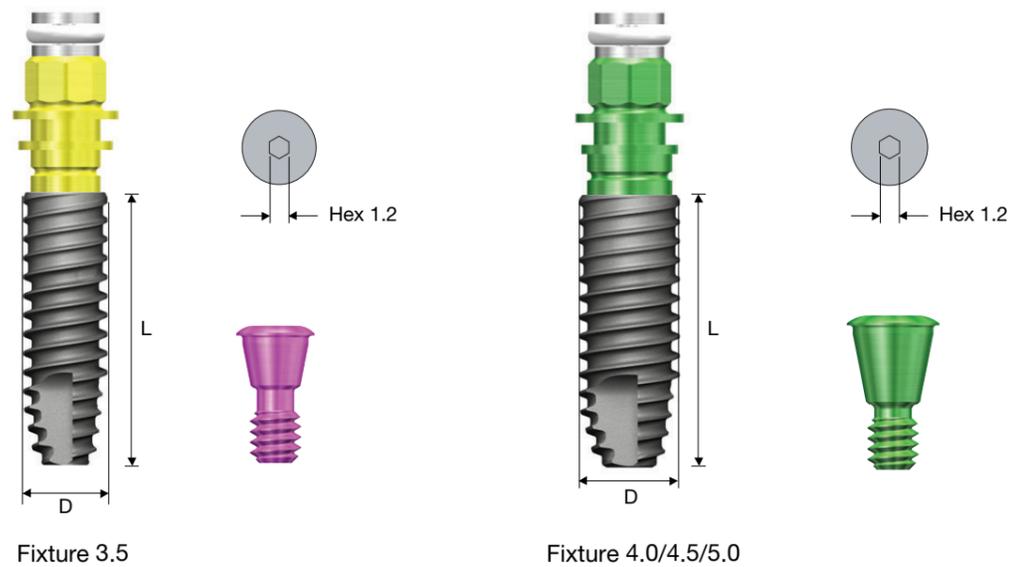

TSII Fixture Order Code

Fixture Only



- Fixture : Product Code [ex : TS2S4010S]

Pre-Mounted Fixture [Simple Mount]

- Fixture + Mount + Cover Screw : B + Product Code [ex : BTS2S4010S]

Feature of TSII Fixture

- Internal Hex & 11° Morse taper connected, submerged fixture
- SA surface morphology and roughness increased by 45% compared to RBM treatment.
- SA : Sand blasted with alumina and Acid etched surface
 - Optimal morphology : Combination of crater and micro-pit
 - Optimal surface roughness : Ra 2.5~3.0 μ m
 - Early cell response : 20% faster than RBM
 - Early bone healing : 20% faster than RBM
 - Early loading possible after 6 weeks of placement.
 - Optimized design for SA surface
- Straight body offers good implantation performance
- Small Thread : Increase initial stability in soft bone
- Corkscrew thread : Powerful Self threading
- Limited insertion torque : 40Ncm

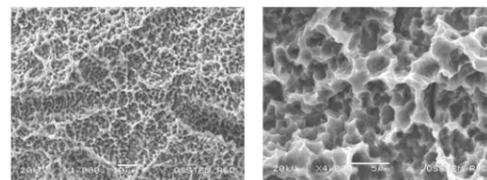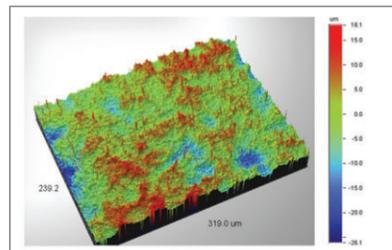


※ We recommend that the fixture with over 4.5mm diameter is used for single case in Molar.


M R Connection

GLOBAL STANDARD OSSTEM IMPLANT


※ The following labeled dimension may differ from the actual dimension.

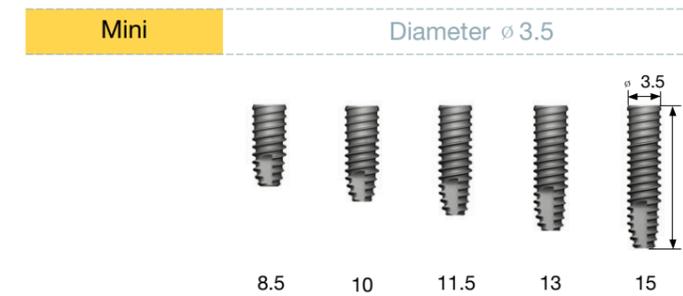


| Connection | | Mini |
|------------|---|------------|
| L | D | ϕ 3.5 |
| 7 | | - |
| 8.5 | | TS2M3508S |
| 10 | | TS2M3510S |
| 11.5 | | TS2M3511S |
| 13 | | TS2M3513S |
| 15 | | TS2M3515S |

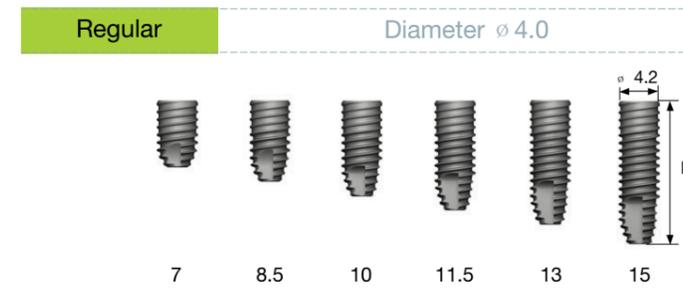

| Connection | | Regular |
|------------|---|------------|
| L | D | ϕ 4.0 |
| 7 | | TS2S4007S |
| 8.5 | | TS2S4008S |
| 10 | | TS2S4010S |
| 11.5 | | TS2S4011S |
| 13 | | TS2S4013S |
| 15 | | TS2S4015S |

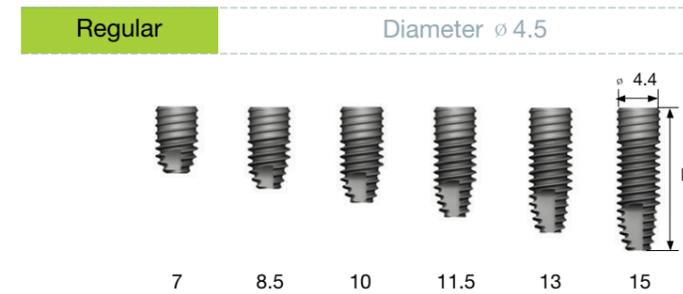


| Connection | | Regular |
|------------|---|------------|
| L | D | ϕ 4.5 |
| 7 | | TS2S4507S |
| 8.5 | | TS2S4508S |
| 10 | | TS2S4510S |
| 11.5 | | TS2S4511S |
| 13 | | TS2S4513S |
| 15 | | TS2S4515S |

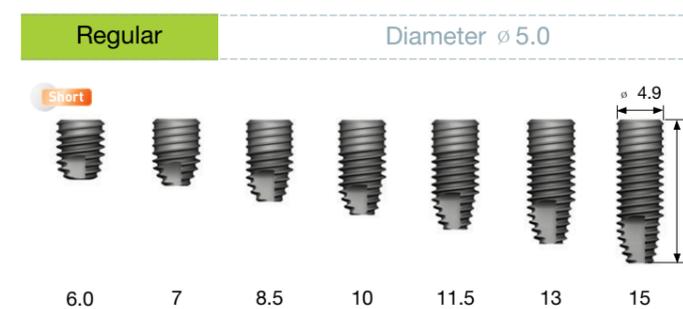

| Connection | | Regular |
|------------|---|------------|
| L | D | ϕ 5.0 |
| 6 | | TS2S5006S |
| 7 | | TS2S5007S |
| 8.5 | | TS2S5008S |
| 10 | | TS2S5010S |
| 11.5 | | TS2S5011S |
| 13 | | TS2S5013S |
| 15 | | TS2S5015S |

※ Note : Short implant require sufficient curing period and, in the process of prosthesis, should be used splinting with another implant.

TSIII Fixture

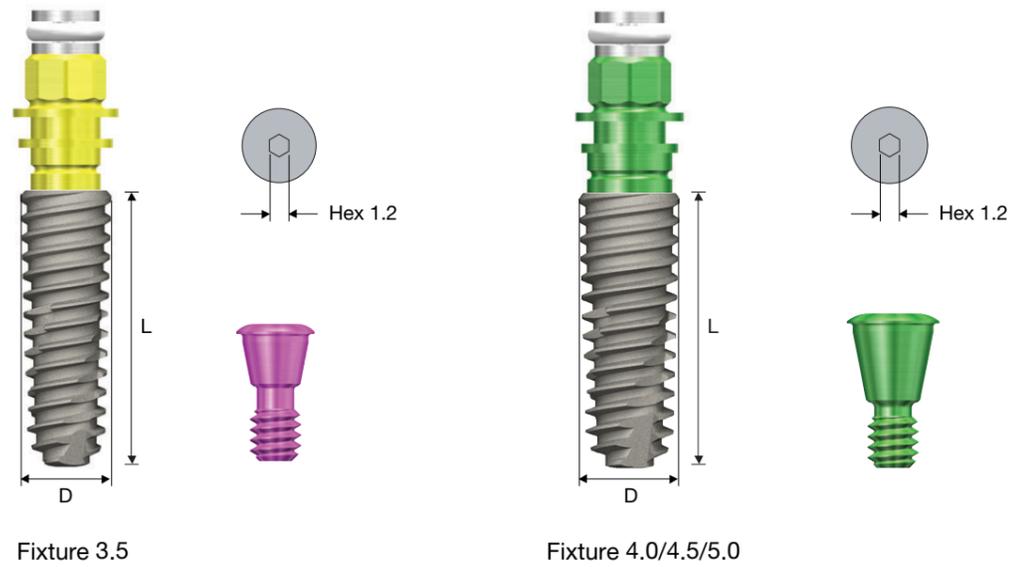

TSIII Fixture Order Code

Fixture Only



- Fixture : Product Code [ex : TS3S4010S]

Pre-Mounted Fixture [Simple Mount]

- Fixture + Mount + Cover Screw : B + Product Code [ex : BTS3S4010S]


Feature of TSIII Fixture

- Internal Hex & 11° Morse taper connected, submerged fixture
- SA surface morphology and roughness increased by 45% compared to RBM treatment.
- SA : Sand blasted with alumina and Acid etched surface
 - Optimal morphology : Combination of crater and micro-pit
 - Optimal surface roughness : Ra 2.5~3.0 μ m
 - Early cell response : 20% faster than RBM
 - Early bone healing : 20% faster than RBM
 - Early loading possible after 6 weeks of placement.
 - Optimized design for SA surface
- Taper body offers High initial stability
- Small Thread : Increase initial stability in soft bone
- Corkscrew thread : Powerful Self threading
- Limited insertion torque : 40Ncm

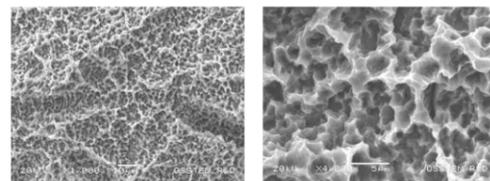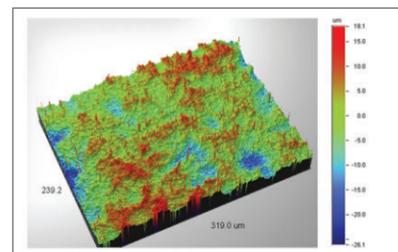


※ We recommend that the fixture with over 4.5mm diameter is used for single case in Molar.


※ The following labeled dimension may differ from the actual dimension.

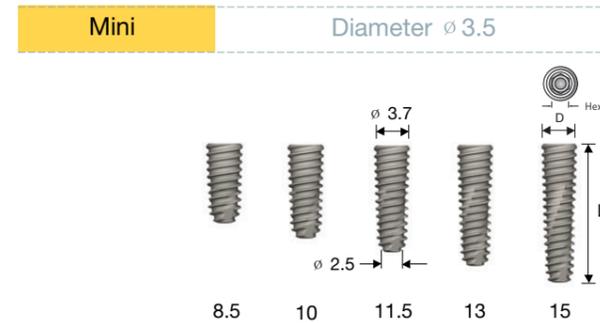


| Connection | Mini |
|------------|------------|
| L \ D | ϕ 3.5 |
| 7 | - |
| 8.5 | TS3M3508S |
| 10 | TS3M3510S |
| 11.5 | TS3M3511S |
| 13 | TS3M3513S |
| 15 | TS3M3515S |

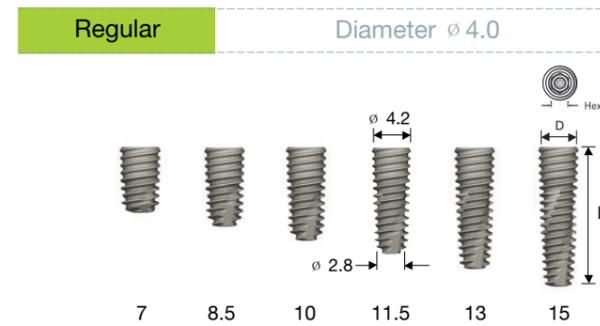

| Connection | Regular |
|------------|------------|
| L \ D | ϕ 4.0 |
| 7 | TS3S4007S |
| 8.5 | TS3S4008S |
| 10 | TS3S4010S |
| 11.5 | TS3S4011S |
| 13 | TS3S4013S |
| 15 | TS3S4015S |

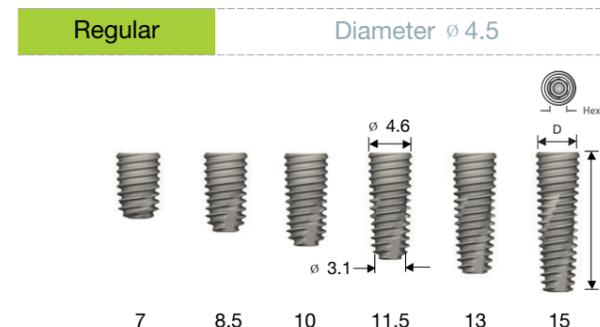


| Connection | Regular |
|------------|------------|
| L \ D | ϕ 4.5 |
| 7 | TS3S4507S |
| 8.5 | TS3S4508S |
| 10 | TS3S4510S |
| 11.5 | TS3S4511S |
| 13 | TS3S4513S |
| 15 | TS3S4515S |

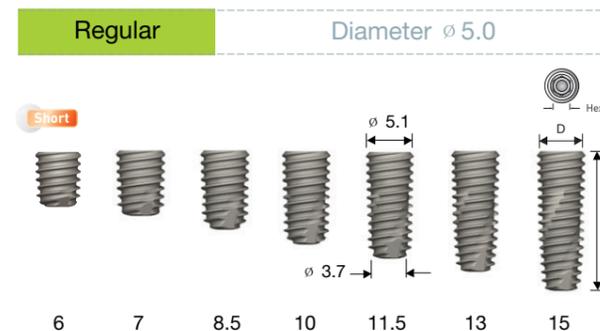

| Connection | Regular |
|------------|------------|
| L \ D | ϕ 5.0 |
| 6 | TS3S5006S |
| 7 | TS3S5007S |
| 8.5 | TS3S5008S |
| 10 | TS3S5010S |
| 11.5 | TS3S5011S |
| 13 | TS3S5013S |
| 15 | TS3S5015S |

※ Note : Short implant require sufficient curing period and, in the process of prosthesis, should be used splinting with another implant.

TSIII Ultra - Wide® Fixture

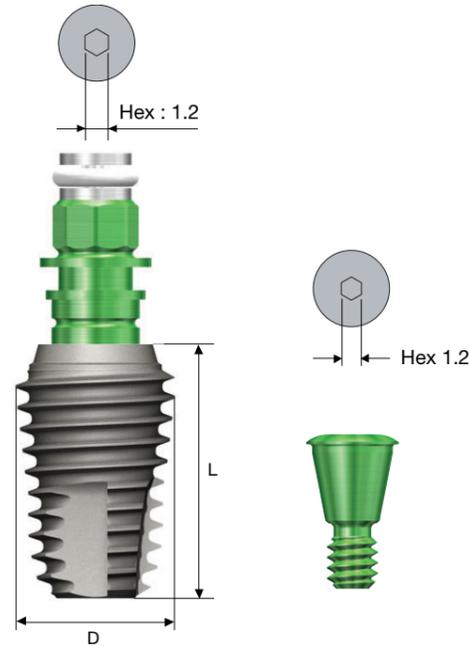

(*Uses the same mount and cover screw with GS Regular)

TSIII Ultra - Wide® Fixture Order Code

Fixture Only



- Fixture : Product Code (예) : TS3S6010S)

Pre-Mounted Fixture (Simple Mount)

- Fixture + Simple Mount + Cover Screw : B + Fixture Product Code (ex : BTS3S6010S)

Feature of TSIII Ultra-Wide® Fixture


- Internal Hex & 11° morse taper connected, submerged fixture
- SA surface morphology and roughness increased by 45% compared to RBM treatment.
- SA : Sand blasted with alumina and Acid etched surface
 - Optimal morphology : Combination of crater and micro-pit
 - Optimal surface roughness : Ra 2.5~3.0 μm
 - Early cell response : 20% faster than RBM
 - Early bone healing : 20% faster than RBM
 - Early loading possible after 6 weeks of placement.
- Compatible with GS Regular abutment components
- A fixture that is convenient to use in case of immediate installation following posterior tooth extract socket and replacement of failed implant
- Optimized apex design that enables gaining stable initial fixture even at 3 mm below the extract socket
- 4-bladed cutting edge with excellent self-tapping force
- Limited insertion torque : 40Ncm

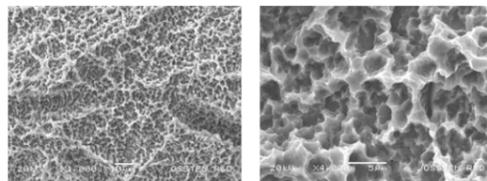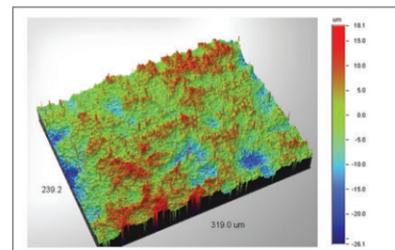


R Connection

GLOBAL STANDARD OSSTEM IMPLANT

※ The following labeled dimension may differ from the actual dimension.

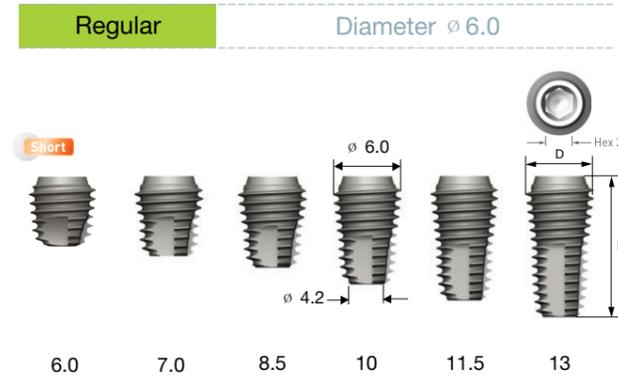


| Connection | | Regular |
|------------|------|------------|
| L | D | ϕ 6.0 |
| | | |
| | 6 | TS3S6006S |
| | 7 | TS3S6007S |
| | 8.5 | TS3S6008S |
| | 10 | TS3S6010S |
| | 11.5 | TS3S6011S |
| | 13 | TS3S6013S |

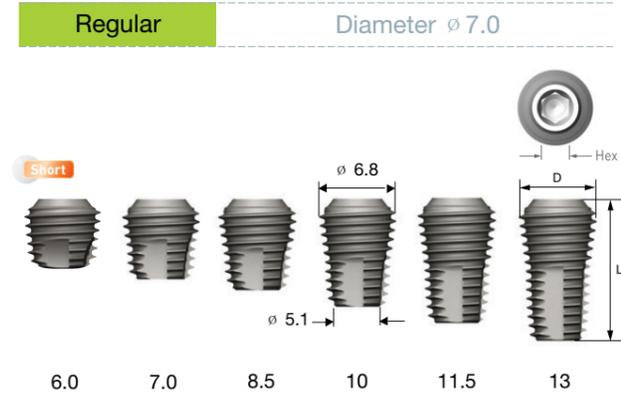

| Connection | | Regular |
|------------|------|------------|
| L | D | ϕ 7.0 |
| | | |
| | 6 | TS3S7006S |
| | 7 | TS3S7007S |
| | 8.5 | TS3S7008S |
| | 10 | TS3S7010S |
| | 11.5 | TS3S7011S |
| | 13 | TS3S7013S |

※ Note : Short implant require sufficient curing period and, in the process of prosthesis, should be used splinting with another implant.

TSIV Fixture

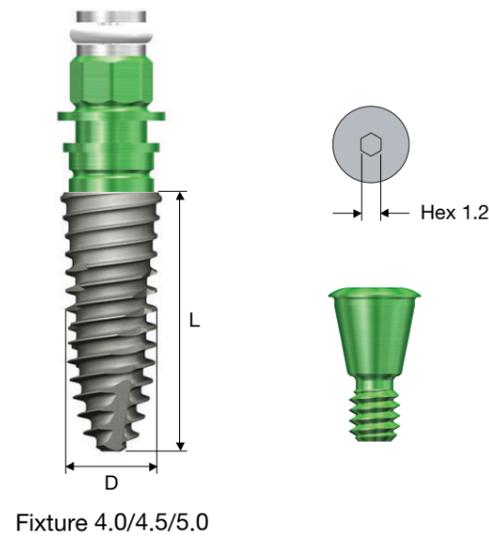

TSIV Fixture Order Code

Fixture Only



- Fixture : Product Code [ex : TS4S4010S]

Pre-Mounted Fixture [Simple Mount]

- Fixture + Mount + Cover Screw : B + Product Code [ex : BTS4S4010S]

Feature of TSIV Fixture

- Internal Hex & 11° morse taper connected, submerged fixture
- SA surface morphology and roughness increased by 45% compared to RBM treatment.
- SA : Sand blasted with alumina and Acid etched surface
 - Optimal morphology : Combination of crater and micro-pit
 - Optimal surface roughness : Ra 2.5~3.0 μ m
 - Early cell response : 20% faster than RBM
 - Early bone healing : 20% faster than RBM
 - Early loading possible after 6 weeks of placement.
- Compatible with GS Regular abutment components
- Optimized design for SA surface
- Sinus and soft bone only used fixture
- Small Thread : Increase initial stability in soft bone
- Sharp Apex design : D4 bone case is possible to insert after ϕ 2, ϕ 3mm drilling depth
- Limited insertion torque : 40Ncm

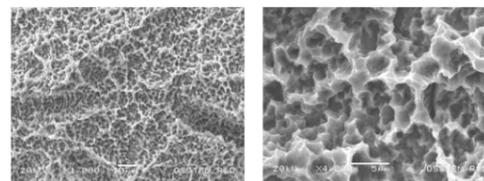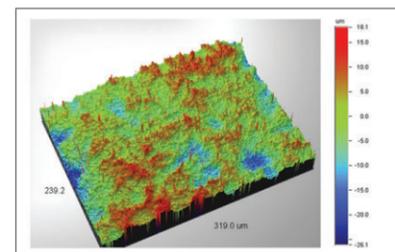


※ We recommend that the fixture with over 4.5mm diameter is used for single case in Molar.

※ Recommended insertion speed : below 15rpm
- TSIV Fixture Insert speed is fast because of thread pitch is big


R Connection

GLOBAL STANDARD OSSTEM IMPLANT


※ The following labeled dimension may differ from the actual dimension.

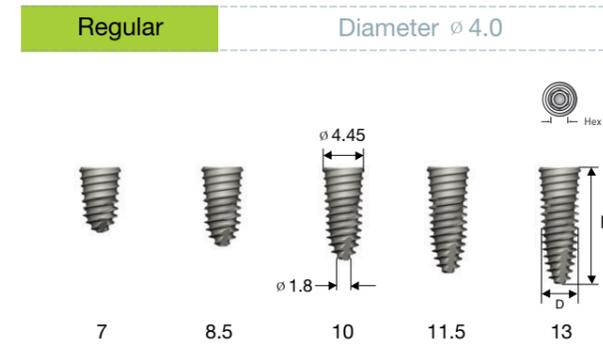

| Connection | Regular |
|------------|-----------------------|
| L \ D | ϕ 4.0(Pitch 0.8) |
| 7 | TS4S4007S |
| 8.5 | TS4S4008S |
| 10 | TS4S4010S |
| 11.5 | TS4S4011S |
| 13 | TS4S4013S |

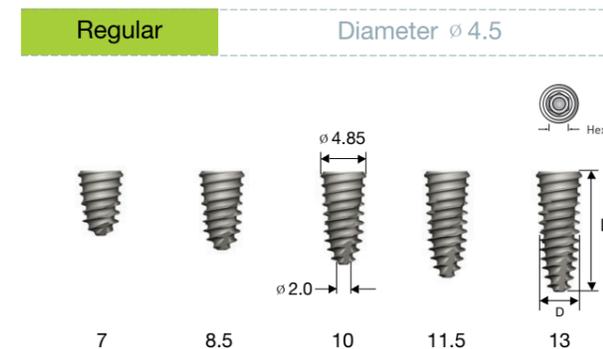


| Connection | Regular |
|------------|-----------------------|
| L \ D | ϕ 4.5(Pitch 1.0) |
| 7 | TS4S4507S |
| 8.5 | TS4S4508S |
| 10 | TS4S4510S |
| 11.5 | TS4S4511S |
| 13 | TS4S4513S |

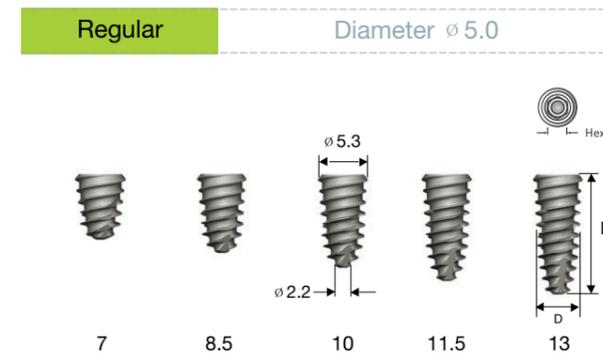

| Connection | Regular |
|------------|-----------------------|
| L \ D | ϕ 5.0(Pitch 1.2) |
| 7 | TS4S5007S |
| 8.5 | TS4S5008S |
| 10 | TS4S5010S |
| 11.5 | TS4S5011S |
| 13 | TS4S5013S |

GSII RBM Fixture

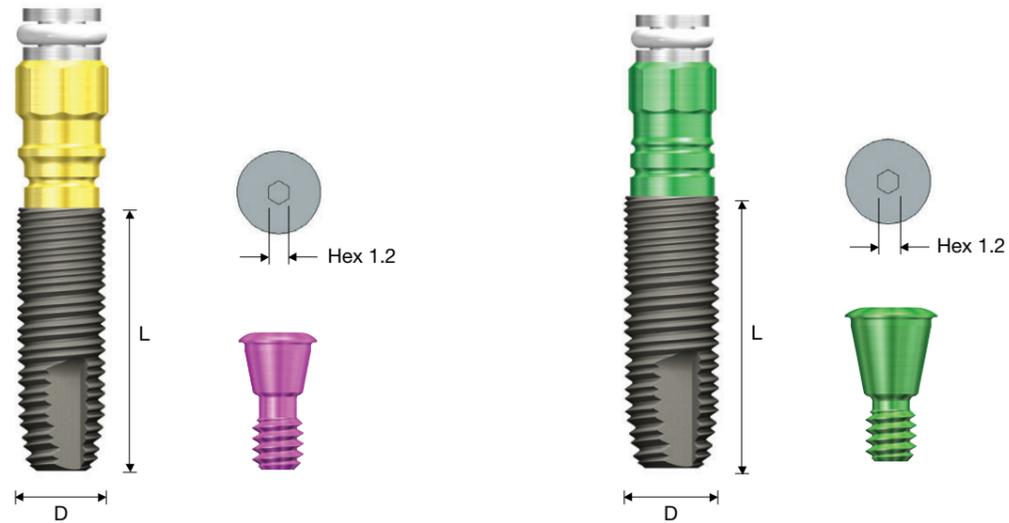

GSII RBM Fixture Order Code

Fixture Only

- Fixture : Product Code (Ex : GS2R4011R01)

Pre-Mounted Fixture (Simple Mount)

- Fixture + Simple Mount + Cover Screw : B + Fixture Product Code (Ex : BGS2R4011R01)

Features of GSII RBM Fixture

- Internal hex & 11° morse taper connected, submerged fixture
- Harmony of macro thread and micro thread considering the cortical and cancellous bone
- Dual thread design offers excellent initial bonding and long-term stability
- RBM : Excellent bio-affinity of surface
- Rigid motion with superstructure helps maintain stable connection
- Straight body facilitates the adjustment of implantation depth
- 3-bladed cutting edge with excellent self-tapping force
- A variety of diameters and lengths are available for various oral environments
- Limited insertion torque : 40Ncm


※ We recommend that the fixture with over 4.5mm diameter is used for single case in Molar.

M R Connection


GLOBAL STANDARD OSSTEM IMPLANT

※ The following labeled dimension may differ from the actual dimension.


Mini Diameter ϕ 3.5

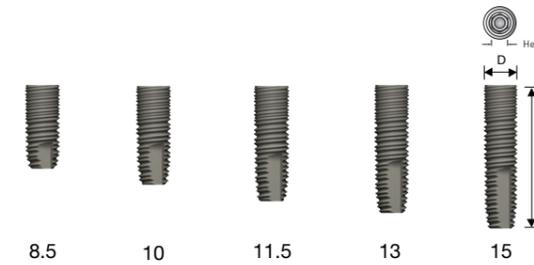


Regular Diameter ϕ 4.0

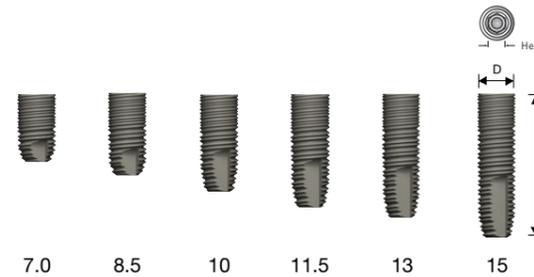

Regular Diameter ϕ 4.5

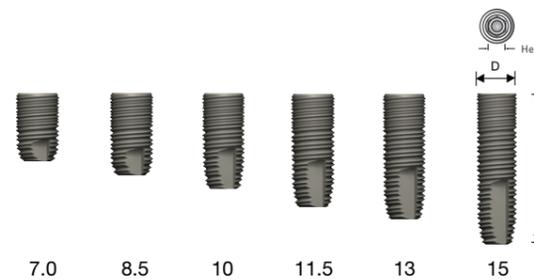

Regular Diameter ϕ 5.0

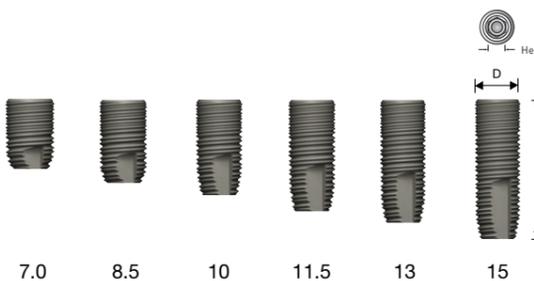


| Connection | | Mini |
|------------|-------------|------------|
| D | | ϕ 3.5 |
| L | RBM | |
| 7 | - | |
| 8.5 | GS2M3508R01 | |
| 10 | GS2M3510R01 | |
| 11.5 | GS2M3511R01 | |
| 13 | GS2M3513R01 | |
| 15 | GS2M3515R01 | |

| Connection | | Regular |
|------------|-------------|------------|
| D | | ϕ 4.0 |
| L | RBM | |
| 7 | GS2R4007R01 | |
| 8.5 | GS2R4008R01 | |
| 10 | GS2R4010R01 | |
| 11.5 | GS2R4011R01 | |
| 13 | GS2R4013R01 | |
| 15 | GS2R4015R01 | |

| Connection | | Regular |
|------------|-------------|------------|
| D | | ϕ 4.5 |
| L | RBM | |
| 7 | GS2W4507R01 | |
| 8.5 | GS2W4508R01 | |
| 10 | GS2W4510R01 | |
| 11.5 | GS2W4511R01 | |
| 13 | GS2W4513R01 | |
| 15 | GS2W4515R01 | |

| Connection | | Regular |
|------------|-------------|------------|
| D | | ϕ 5.0 |
| L | RBM | |
| 7 | GS2W5007R01 | |
| 8.5 | GS2W5008R01 | |
| 10 | GS2W5010R01 | |
| 11.5 | GS2W5011R01 | |
| 13 | GS2W5013R01 | |
| 15 | GS2W5015R01 | |

GSII RBM Ultra - Wide® Fixture

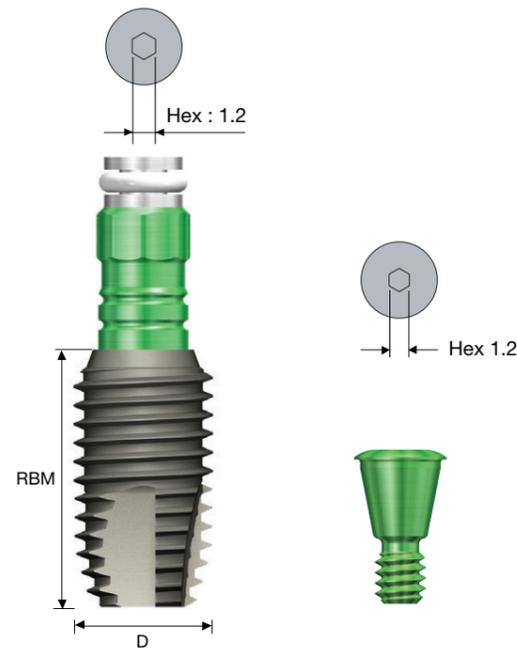

(*Uses the same mount and cover screw with GS Regular)

GSII RBM Ultra - Wide® Fixture Order Code

Fixture Only

- Fixture : Product Code (ex : GS2W6010R02)

Pre-Mounted Fixture (Simple Mount)

- Fixture + Simple Mount + Cover Screw : B + Fixture Product Code (ex : BGS2W6010R02)


Features of GSII RBM Ultra - Wide® Fixture

- Internal hex & 11° morse taper connected, submerged wide diameter fixture
- Compatible with GS Regular abutment components
- A fixture that is convenient to use in case of immediate installation following posterior tooth extract socket and replacement of failed implants
- Optimized apex design that enables gaining stable initial fixation even at 3 mm below the extract socket
- All RBM surfaces with excellent bio-affinity
- Rigid motion with superstructure helps maintain stable connection
- 4-bladed cutting edge with excellent self-tapping force
- A variety of diameters and lengths are available for various oral environments
- Limited insertion torque : 40 Ncm


R Connection

GLOBAL STANDARD OSSTEM IMPLANT

※ The following labeled dimension may differ from the actual dimension.

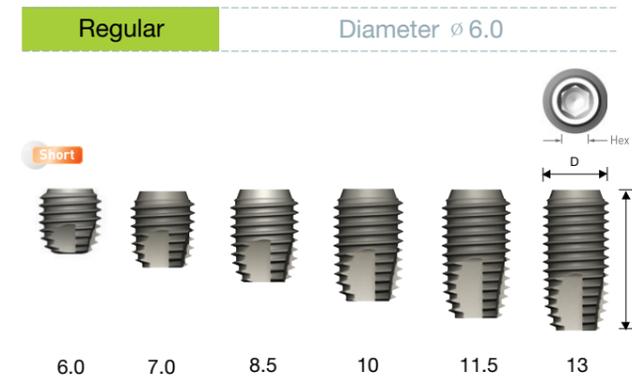

| Connection | | Regular |
|-------------|---|-------------|
| L | D | ø 6.0 |
| 6.0 (Short) | | GS2W6006R02 |
| 7.0 | | GS2W6007R02 |
| 8.5 | | GS2W6008R02 |
| 10 | | GS2W6010R02 |
| 11.5 | | GS2W6011R02 |
| 13 | | GS2W6013R02 |

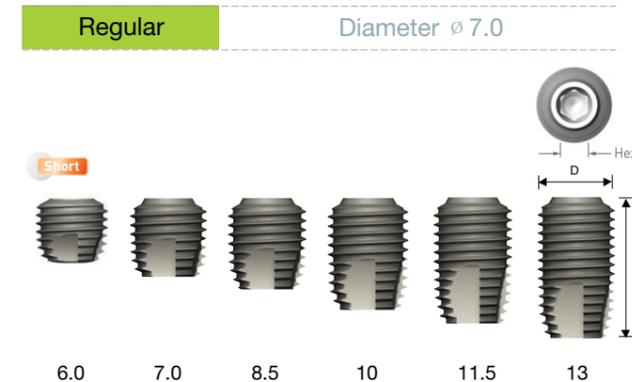


| Connection | | Regular |
|-------------|---|-------------|
| L | D | ø 7.0 |
| 6.0 (Short) | | GS2W7006R02 |
| 7.0 | | GS2W7007R02 |
| 8.5 | | GS2W7008R02 |
| 10 | | GS2W7010R02 |
| 11.5 | | GS2W7011R02 |
| 13 | | GS2W7013R02 |

* The actual length of GSII Ultra-Wide® Fixture is L-0.5mm. (Except for length 7mm)

※ Note : Short implant require sufficient curing period and, in the process of prosthesis, should be used splinting with another implant.

GSIII RBM Fixture

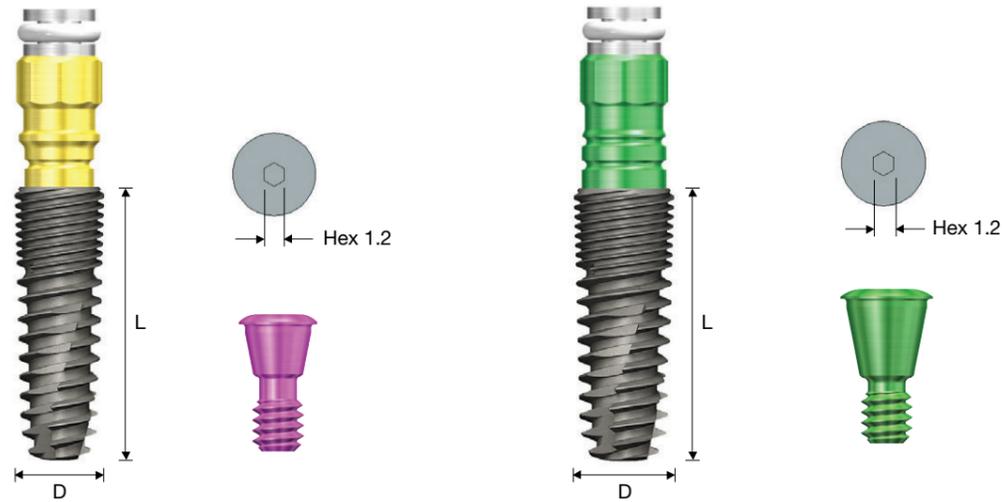

GSIII Fixture 3.5

GSIII Fixture 4.0/4.5/5.0

GSIII RBM Fixture Order Code

Fixture Only

- Fixture : Product Code [ex : GS3S4011R]

Pre-Mounted Fixture [Simple Mount]

- Fixture + Mount + Cover Screw : B + Product Code [ex : BGS3S4011R]

Feature of GSIII RBM Fixture


- Internal hex & 11° morse taper connected, submerged fixture
- Taper body offers excellent primary bonding
- Micro Thread
 - Distribute stress on bone
 - Stimulate bone evenly
 - Increase cell response
 - Reinforce fixture strength
- Corkscrew Thread & Cutting Edge
 - Powerful self threading
 - Change path easily
 - Increase insertion torque in soft bone
 - Increase initial stability in soft bone
- Rigid motion with superstructure helps maintain stable connection
- A variety of diameters and lengths are available for various oral environments
- Limited insertion torque : 40Ncm

※ We recommend that the fixture with over 4.5mm diameter is used for single case in Molar.


M R Connection

GLOBAL STANDARD OSSTEM IMPLANT


※ The following labeled dimension may differ from the actual dimension.

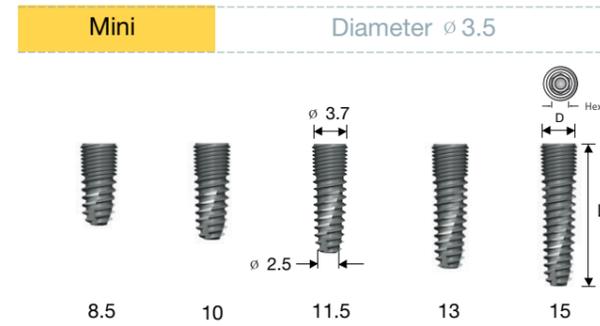


| Connection | | Mini |
|------------|------|------------|
| L | D | ϕ 3,5 |
| | | |
| | 7 | - |
| | 8.5 | GS3M3508R |
| | 10 | GS3M3510R |
| | 11.5 | GS3M3511R |
| | 13 | GS3M3513R |
| | 15 | GS3M3515R |

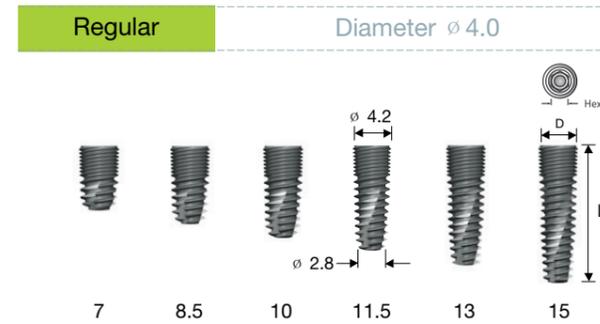

| Connection | | Regular |
|------------|------|------------|
| L | D | ϕ 4,0 |
| | | |
| | 7 | GS3S4007R |
| | 8.5 | GS3S4008R |
| | 10 | GS3S4010R |
| | 11.5 | GS3S4011R |
| | 13 | GS3S4013R |
| | 15 | GS3S4015R |

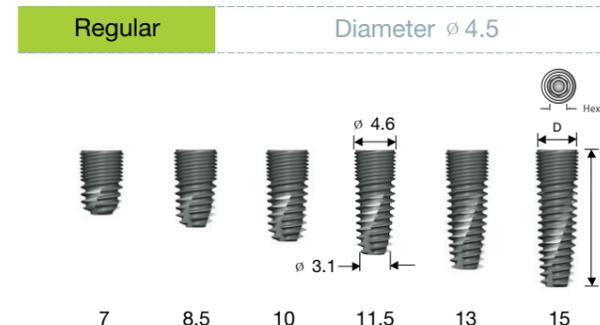

| Connection | | Regular |
|------------|------|------------|
| L | D | ϕ 4,5 |
| | | |
| | 7 | GS3S4507R |
| | 8.5 | GS3S4508R |
| | 10 | GS3S4510R |
| | 11.5 | GS3S4511R |
| | 13 | GS3S4513R |
| | 15 | GS3S4515R |

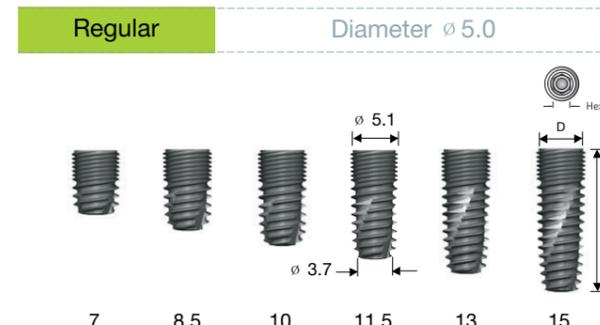

| Connection | | Regular |
|------------|------|------------|
| L | D | ϕ 5,0 |
| | | |
| | 7 | GS3S5007R |
| | 8.5 | GS3S5008R |
| | 10 | GS3S5010R |
| | 11.5 | GS3S5011R |
| | 13 | GS3S5013R |
| | 15 | GS3S5015R |

Simple Mount



| Color | Yellow | Green |
|---------|-------------------|-----------------------------------|
| Fixture | ∅ 3.5 | ∅ 4.0, ∅ 4.5, ∅ 5.0, ∅ 6.0, ∅ 7.0 |
| Code | GISMY-3015A GSSMY | GISMG-3512A GSSSG |


- Color indication facilitates easy identification in the oral cavity
 ∅ 3.5 : Yellow,
 ∅ 4.0, ∅ 4.5, ∅ 5.0, ∅ 6.0, ∅ 7.0 : Green
- Use a 1.2 hex driver to remove screws
- Packing unit : Mount + Mount Screw
- Tightening torque : 8-10Ncm

Cover Screw




| Color | Purple | Green |
|---------|----------------|-----------------------------------|
| Fixture | ∅ 3.5 | ∅ 4.0, ∅ 4.5, ∅ 5.0, ∅ 6.0, ∅ 7.0 |
| Code | GSCS35 GSCS35L | GSCS40S-G GSCS40L-G |

- Color to easily distinguish the locations of the implemented fixtures
 ∅ 3.5 fixture : Purple
 ∅ 4.0, ∅ 4.5, ∅ 5.0 fixture : Green
- Use a long cover screw when fixture implanted under the bone level
 ∅ 3.5 Fixture : Green
 ∅ 4.0/ ∅ 4.5/ ∅ 5.0/ ∅ 6.0/ ∅ 7.0 : Blue
- Use a 1.2 hex driver
- Packing unit : Cover screw
- Tightening torque : 5-8 Ncm

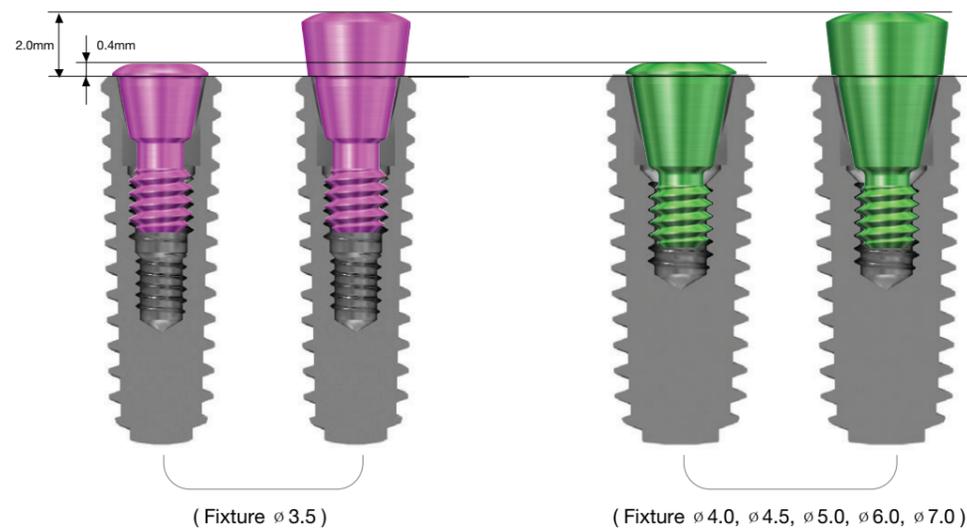

Healing Abutment


Mini

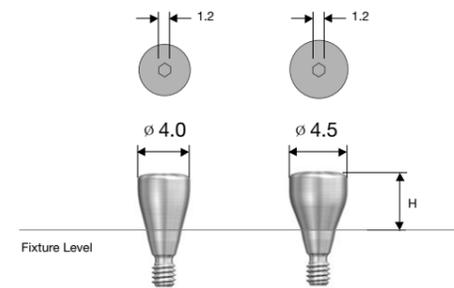

| | | Mini | | | |
|-------|---|----------|----------|----------|----------|
| D | H | 3.0 | 4.0 | 5.0 | 7.0 |
| ∅ 4.0 | | TSHA403M | TSHA404M | TSHA405M | TSHA407M |
| ∅ 4.5 | | TSHA453M | TSHA454M | TSHA455M | TSHA457M |

- Use a 1.2 hex driver
- Packing unit : Healing abutment
- Tightening torque : Hand tightening (less than 10Ncm)

Regular

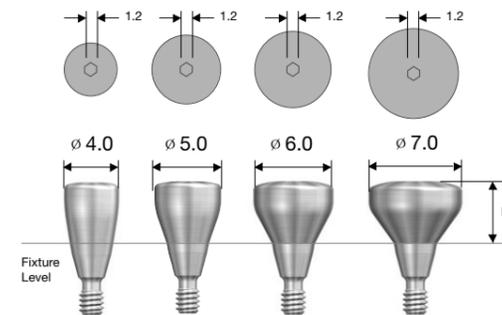



| | | Regular | | | |
|-------|---|----------|----------|----------|----------|
| D | H | 3.0 | 4.0 | 5.0 | 7.0 |
| ∅ 4.0 | | TSHA403R | TSHA404R | TSHA405R | TSHA407R |
| ∅ 5.0 | | TSHA503R | TSHA504R | TSHA505R | TSHA507R |
| ∅ 6.0 | | TSHA603R | TSHA604R | TSHA605R | TSHA607R |
| ∅ 7.0 | | TSHA703R | TSHA704R | TSHA705R | TSHA707R |

※ Matching Table for Healing ABT. & Abutment

| | | | | |
|------------------|---|--------|--------|-------------|
| Healing ABT. (H) | 3 | 4 | 5 | 7 |
| Abutment (G/H) | 1 | 2 or 3 | 3 or 4 | More than 5 |

OSSTEM Implant System


Early & Esthetic OSSTEM IMPLANT

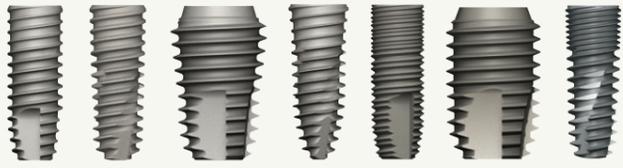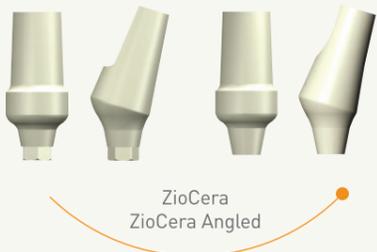

TS & GS System

Components Guide

Compatibility Guide for TS & GS System (Fixture-Abutment)

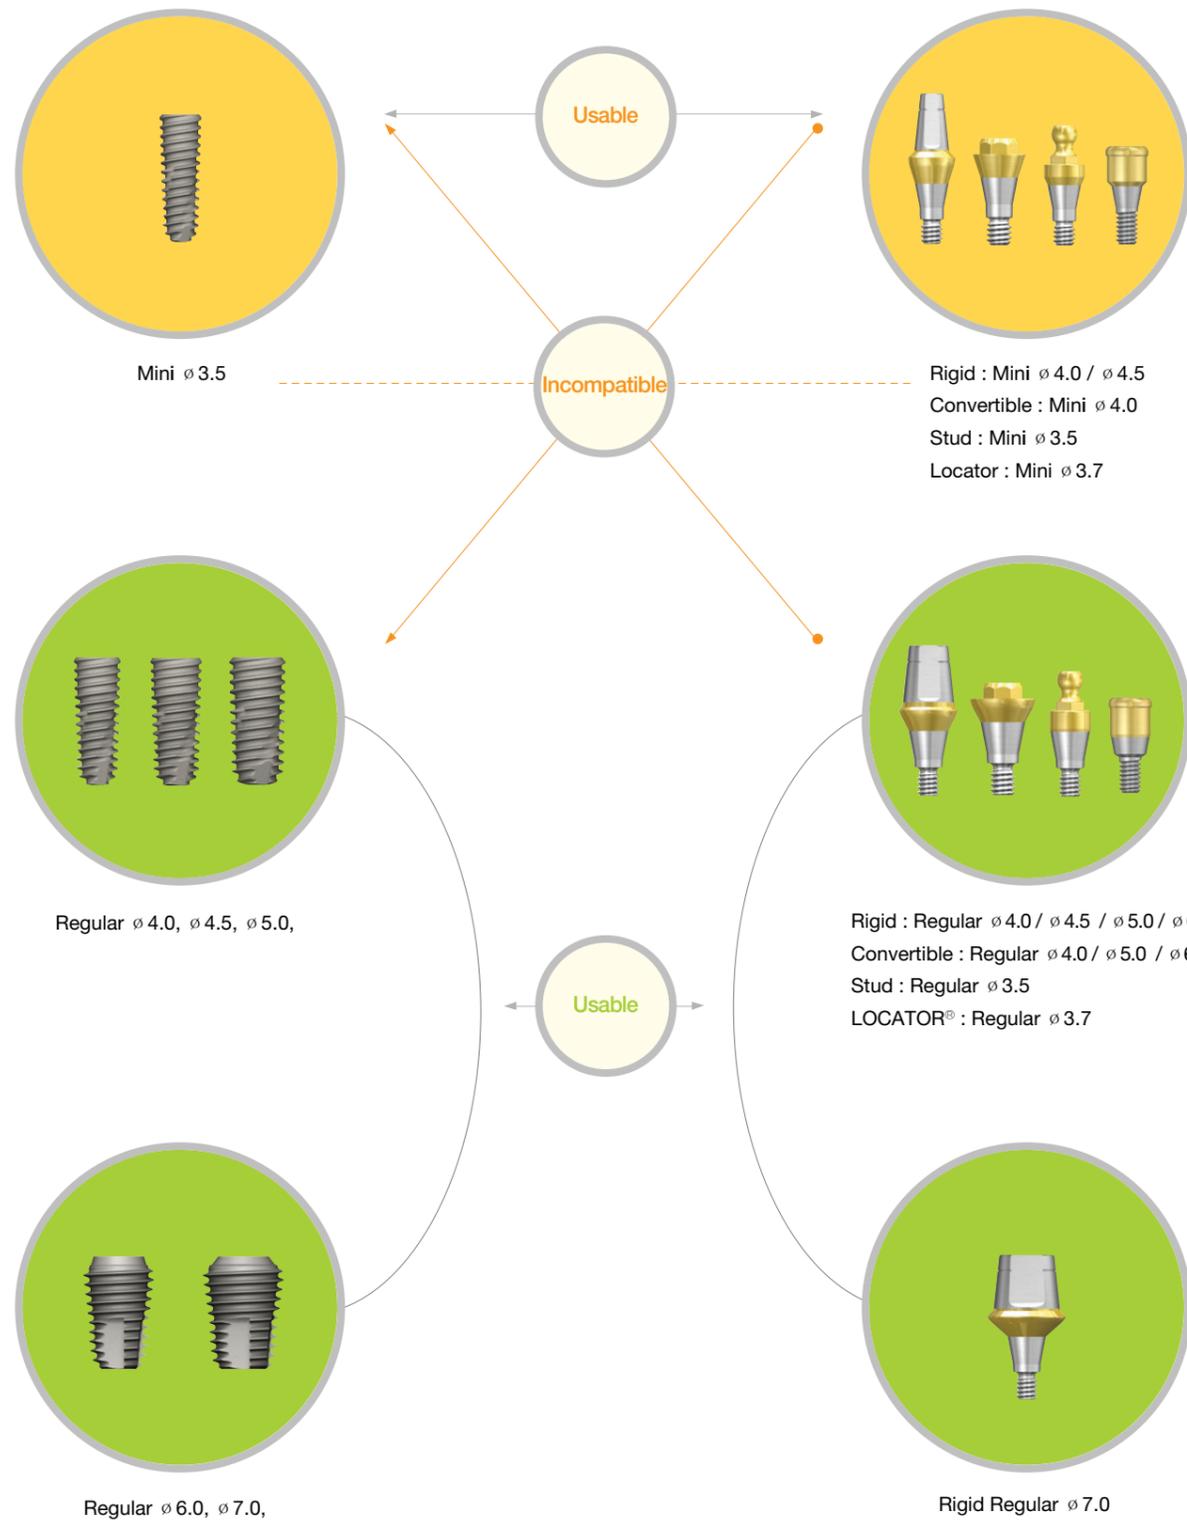


Rigid Abutment Components


Rigid Abutment Cement Retained Restoration

Mini


ø 4.0

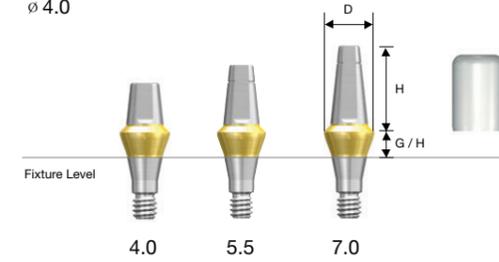

ø 4.5

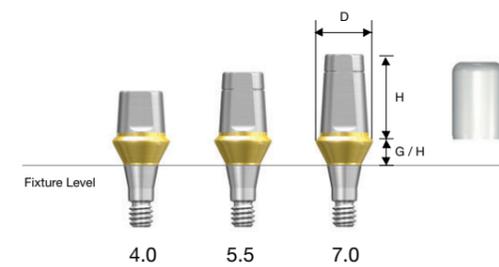

| H | D | | ø 4.0 | ø 4.5 |
|-----|-----|--|----------|----------|
| | G/H | | | |
| 4.0 | 1.0 | | GSRA4410 | GSRA4411 |
| | 2.0 | | GSRA4420 | GSRA4421 |
| | 3.0 | | GSRA4430 | GSRA4431 |
| | 4.0 | | GSRA4440 | GSRA4441 |
| | 5.0 | | GSRA4450 | GSRA4451 |
| 5.5 | 1.0 | | GSRA4610 | GSRA4611 |
| | 2.0 | | GSRA4620 | GSRA4621 |
| | 3.0 | | GSRA4630 | GSRA4631 |
| | 4.0 | | GSRA4640 | GSRA4641 |
| | 5.0 | | GSRA4650 | GSRA4651 |
| 7.0 | 1.0 | | GSRA4710 | GSRA4711 |
| | 2.0 | | GSRA4720 | GSRA4721 |
| | 3.0 | | GSRA4730 | GSRA4731 |
| | 4.0 | | GSRA4740 | GSRA4741 |
| | 5.0 | | GSRA4750 | GSRA4751 |

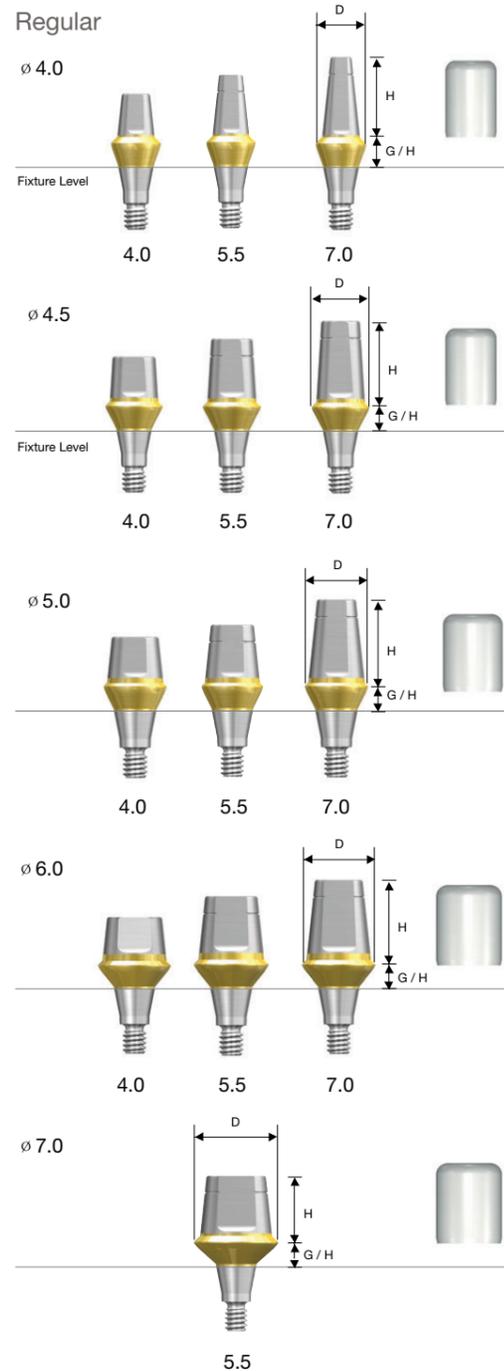

| H | G/H | D | ø 4.0 | ø 4.5 | ø 5.0 |
|-----|-----|---|-----------|-----------|----------|
| 4.0 | 1.0 | | GSRAS4410 | GSRAS4411 | GSRA5410 |
| | 2.0 | | GSRAS4420 | GSRAS4421 | GSRA5420 |
| | 3.0 | | GSRAS4430 | GSRAS4431 | GSRA5430 |
| | 4.0 | | GSRAS4440 | GSRAS4441 | GSRA5440 |
| | 5.0 | | GSRAS4450 | GSRAS4451 | GSRA5450 |
| 5.5 | 1.0 | | GSRAS4610 | GSRAS4611 | GSRA5610 |
| | 2.0 | | GSRAS4620 | GSRAS4621 | GSRA5620 |
| | 3.0 | | GSRAS4630 | GSRAS4631 | GSRA5630 |
| | 4.0 | | GSRAS4640 | GSRAS4641 | GSRA5640 |
| | 5.0 | | GSRAS4650 | GSRAS4651 | GSRA5650 |
| 7.0 | 1.0 | | GSRAS4710 | GSRAS4711 | GSRA5710 |
| | 2.0 | | GSRAS4720 | GSRAS4721 | GSRA5720 |
| | 3.0 | | GSRAS4730 | GSRAS4731 | GSRA5730 |
| | 4.0 | | GSRAS4740 | GSRAS4741 | GSRA5740 |
| | 5.0 | | GSRAS4750 | GSRAS4751 | GSRA5750 |
| H | G/H | D | ø 6.0 | ø 7.0 | |
| 4.0 | 1.0 | | GSRA6410 | - | |
| | 2.0 | | GSRA6420 | - | |
| | 3.0 | | GSRA6430 | - | |
| | 4.0 | | GSRA6440 | - | |
| | 5.0 | | GSRA6450 | - | |
| 5.5 | 1.0 | | GSRA6610 | GSRA7610 | |
| | 2.0 | | GSRA6620 | GSRA7620 | |
| | 3.0 | | GSRA6630 | GSRA7630 | |
| | 4.0 | | GSRA6640 | GSRA7640 | |
| | 5.0 | | GSRA6650 | GSRA7650 | |
| 7.0 | 1.0 | | GSRA6710 | - | |
| | 2.0 | | GSRA6720 | - | |
| | 3.0 | | GSRA6730 | - | |
| | 4.0 | | GSRA6740 | - | |
| | 5.0 | | GSRA6750 | - | |

- Use for making general cement-type prosthesis
- Abutment and screw in one
- 11° taper connection for excellent safety
- Gingival gold color for aesthetic effect
- Cross-section design for the prevention of prosthesis rotation
- ø 4.0 : Use an outer driver
ø 4.5, ø 5.0, ø 6.0 : Use an outer driver and a 1.2 hex driver
ø 7.0 : Use a 1.2 hex driver
- Packing unit : Abutment + Protect Cap
- Tightening torque : 30 Ncm

Order code - Abutment + Protect cap: Product code + P (ex: GSRA5620P)

Rigid Protect Cap



| | | Mini / Regular | |
|-----|---|----------------|----------|
| H | D | ø 4.0 | ø 4.5 |
| 4.0 | | GSRPC440 | GSRPC441 |
| 5.5 | | GSRPC460 | GSRPC461 |
| 7.0 | | GSRPC470 | GSRPC471 |

| | | Regular | | |
|-----|---|----------|----------|----------|
| H | D | ø 5.0 | ø 6.0 | ø 7.0 |
| 4.0 | | GSRPC540 | GSRPC640 | - |
| 5.5 | | GSRPC560 | GSRPC660 | GSRPC760 |
| 7.0 | | GSRPC570 | GSRPC670 | - |

- Use for the protection of the rigid abutment in the oral cavity and to minimize the patient's discomfort
- Applicable as a substructure of temporary prosthesis
- Convenient locking
- Packing unit : Protect Cap

Rigid Retraction Cap




| | | Mini / Regular | |
|-----|---|----------------|----------|
| H | D | ø 4.0 | ø 4.5 |
| 4.0 | | GSRRC440 | GSRRC441 |
| 5.5 | | GSRRC460 | GSRRC461 |
| 7.0 | | GSRRC470 | GSRRC471 |

| | | Regular | | |
|-----|---|----------|----------|----------|
| H | D | ø 5.0 | ø 6.0 | ø 7.0 |
| 4.0 | | GSRRC540 | GSRRC640 | - |
| 5.5 | | GSRRC560 | GSRRC660 | GSRRC760 |
| 7.0 | | GSRRC570 | GSRRC670 | - |

- Packing unit : Retraction cap
- Possible to take impression in accuracy for margin

Rigid Impression Coping

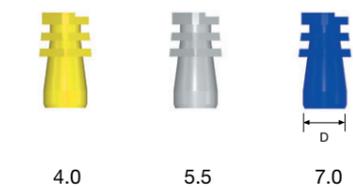


| | | Mini / Regular | |
|-------------|---|----------------|-----------|
| H | D | ø 4.0 | ø 4.5 |
| 4.0(Yellow) | | GSRIC440S | GSRIC441S |
| 5.5(Gray) | | GSRIC460S | GSRIC461S |
| 7.0(Blue) | | GSRIC470S | GSRIC471S |

| | | Regular | | |
|-------------|---|-----------|-----------|-----------|
| H | D | ø 5.0 | ø 6.0 | ø 7.0 |
| 4.0(Yellow) | | GSRIC540S | GSRIC640S | - |
| 5.5(Gray) | | GSRIC560S | GSRIC660S | GSRIC760S |
| 7.0(Blue) | | GSRIC570S | GSRIC670S | - |

- Use for taking an impression of rigid abutments
- Color indication enables the easy identification of abutments of varying lengths 4mm (Yellow), 5.5mm (Gray), 7.0mm (blue)
- Convenient locking
- Packing unit : Impression coping

Rigid Burn-out Cylinder




| | | Mini / Regular | |
|--------|---|----------------|----------|
| Type | D | ø 4.0 | ø 4.5 |
| Single | | GSRP400S | GSRP450S |
| Bridge | | GSRP400B | GSRP450B |

| | | Regular | | |
|--------|---|----------|----------|----------|
| Type | D | ø 5.0 | ø 6.0 | ø 7.0 |
| Single | | GSRP500S | GSRP600S | GSRP700S |
| Bridge | | GSRP500B | GSRP600B | GSRP700B |

- Use as a prosthetic framework by connecting to Rigid Lab analogs
- Color indication facilitates the identification of different cases
Single (Red color), Bridge (White color)
- After prosthetic casting, the margin may be adjusted by a special-purpose reamer
- Packing unit : Burn-out Cylinder

Rigid Lab Analog

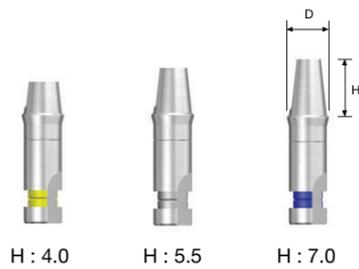


| | | Mini / Regular | |
|-------------|---|----------------|----------|
| H | D | ø 4.0 | ø 4.5 |
| 4.0(Yellow) | | GSRLA440 | GSRLA441 |
| 5.5(Gray) | | GSRLA460 | GSRLA461 |
| 7.0(Blue) | | GSRLA470 | GSRLA471 |

| | | Regular | | |
|-------------|---|----------|----------|----------|
| H | D | ø 5.0 | ø 6.0 | ø 7.0 |
| 4.0(Yellow) | | GSRLA540 | GSRLA640 | - |
| 5.5(Gray) | | GSRLA560 | GSRLA660 | GSRLA760 |
| 7.0(Blue) | | GSRLA570 | GSRLA670 | - |

- Make rigid abutments on a working model
- Color indication enables the easy identification of abutments of varying lengths
4mm (Yellow), 5.5mm (Gray), 7.0mm (blue)
- Packing unit : Lab analog

Transfer Abutment Components

Transfer Abutment - Cement Retained Restoration

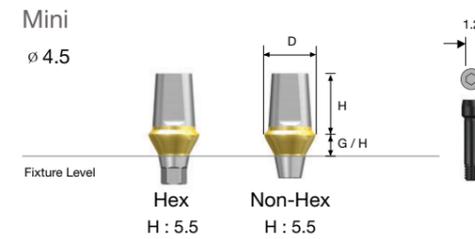


| H | G/H | ø 4.5 | |
|-----------------|-----|----------|-----------|
| | | Hex | Non-Hex |
| 5.5 | 1.0 | GSTA4611 | GSTA4611N |
| | 2.0 | GSTA4621 | GSTA4621N |
| | 3.0 | GSTA4631 | GSTA4631N |
| | 4.0 | GSTA4641 | GSTA4641N |
| | 5.0 | GSTA4651 | GSTA4651N |
| 7.0 | 1.0 | GSTA4711 | GSTA4711N |
| | 2.0 | GSTA4721 | GSTA4721N |
| | 3.0 | GSTA4731 | GSTA4731N |
| | 4.0 | GSTA4741 | GSTA4741N |
| | 5.0 | GSTA4751 | GSTA4751N |
| EbonyGold Screw | | GSABSM | |

- Use for making general cement-type prosthesis
- 11° taper connection for excellent safety
- Gingival gold color for aesthetic effect
- Cross-section design for the prevention of prosthesis rotation
- Use a 1.2 hex driver
- Packing unit : Abutment + EbonyGold screw
- Tightening torque: 20 Ncm (mini), 30 Ncm (regular)


Order code

- Abutment + EbonyGold screw: Product code + WH (ex : GSTA5620WH)

※ Old screw(GSASM, GSASR) is not compatible with the new screw(GSABSM, GSABSS).
Refer to the illustration below, please note the connection.




New ABT VS. Old screw



Old ABT VS. New screw

※ To prevent loosening or fracture retightening (2~3 times) is recommended.



Regular

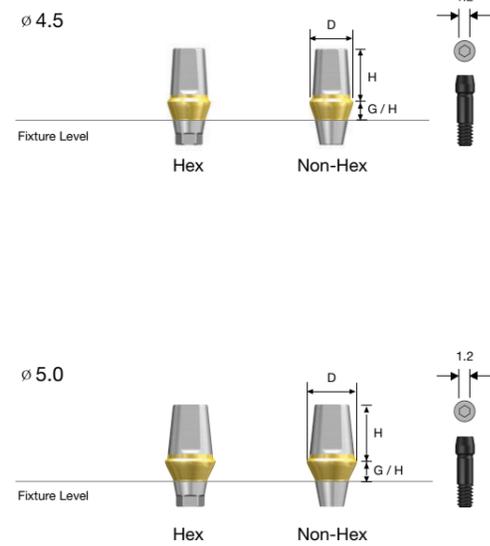

| H | G/H | D | |
|-----------------|-----|-----------|------------|
| | | Hex | Non-Hex |
| ø 4.5 | | | |
| 5.5 | 1.0 | GSTAS4611 | GSTAS4611N |
| | 2.0 | GSTAS4621 | GSTAS4621N |
| | 3.0 | GSTAS4631 | GSTAS4631N |
| | 4.0 | GSTAS4641 | GSTAS4641N |
| | 5.0 | GSTAS4651 | GSTAS4651N |
| 7.0 | 1.0 | GSTAS4711 | GSTAS4711N |
| | 2.0 | GSTAS4721 | GSTAS4721N |
| | 3.0 | GSTAS4731 | GSTAS4731N |
| | 4.0 | GSTAS4741 | GSTAS4741N |
| | 5.0 | GSTAS4751 | GSTAS4751N |
| EbonyGold Screw | | GSABSS | |

| H | G/H | D | |
|-----------------|-----|----------|-----------|
| | | Hex | Non-Hex |
| ø 5.0 | | | |
| 4.0 | 1.0 | GSTA5410 | GSTA5410N |
| | 2.0 | GSTA5420 | GSTA5420N |
| | 3.0 | GSTA5430 | GSTA5430N |
| | 4.0 | GSTA5440 | GSTA5440N |
| | 5.0 | GSTA5450 | GSTA5450N |
| 5.5 | 1.0 | GSTA5610 | GSTA5610N |
| | 2.0 | GSTA5620 | GSTA5620N |
| | 3.0 | GSTA5630 | GSTA5630N |
| | 4.0 | GSTA5640 | GSTA5640N |
| | 5.0 | GSTA5650 | GSTA5650N |
| 7.0 | 1.0 | GSTA5710 | GSTA5710N |
| | 2.0 | GSTA5720 | GSTA5720N |
| | 3.0 | GSTA5730 | GSTA5730N |
| | 4.0 | GSTA5740 | GSTA5740N |
| | 5.0 | GSTA5750 | GSTA5750N |
| EbonyGold Screw | | GSABSS | |


※ A wrong connection may be caused by the incorrect setting of the hex with the fixture hex or interference with bone or adjacent tissue surrounding the installed fixture. The former can be corrected by fixing the hex part setting and checking with an x-ray, and the latter, by removing the interference using tools such as a bone profiler and verifying the exact connection .

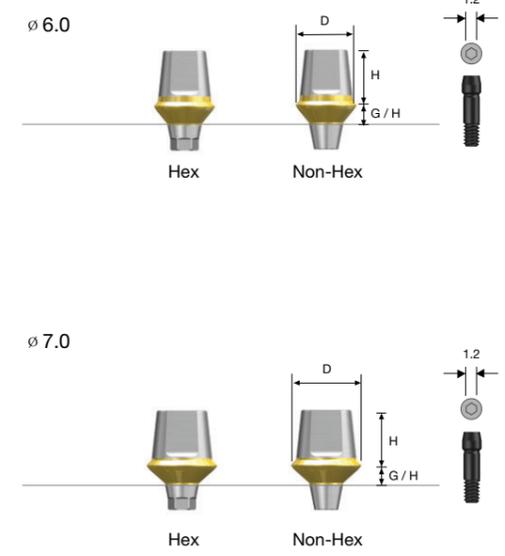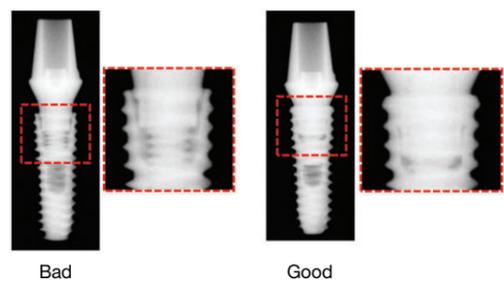

| H | G/H | D | |
|-----------------|-----|----------|-----------|
| | | Hex | Non-Hex |
| ø 6.0 | | | |
| 4.0 | 1.0 | GSTA6410 | GSTA6410N |
| | 2.0 | GSTA6420 | GSTA6420N |
| | 3.0 | GSTA6430 | GSTA6430N |
| | 4.0 | GSTA6440 | GSTA6440N |
| | 5.0 | GSTA6450 | GSTA6450N |
| 5.5 | 1.0 | GSTA6610 | GSTA6610N |
| | 2.0 | GSTA6620 | GSTA6620N |
| | 3.0 | GSTA6630 | GSTA6630N |
| | 4.0 | GSTA6640 | GSTA6640N |
| | 5.0 | GSTA6650 | GSTA6650N |
| 7.0 | 1.0 | GSTA6710 | GSTA6710N |
| | 2.0 | GSTA6720 | GSTA6720N |
| | 3.0 | GSTA6730 | GSTA6730N |
| | 4.0 | GSTA6740 | GSTA6740N |
| | 5.0 | GSTA6750 | GSTA6750N |
| EbonyGold Screw | | GSABSS | |

| H | G/H | D | |
|-----------------|-----|----------|-----------|
| | | Hex | Non-Hex |
| ø 7.0 | | | |
| 5.5 | 1.0 | GSTA7610 | GSTA7610N |
| | 2.0 | GSTA7620 | GSTA7620N |
| | 3.0 | GSTA7630 | GSTA7630N |
| | 4.0 | GSTA7640 | GSTA7640N |
| | 5.0 | GSTA7650 | GSTA7650N |
| EbonyGold Screw | | GSABSS | |

Laboratory Screw

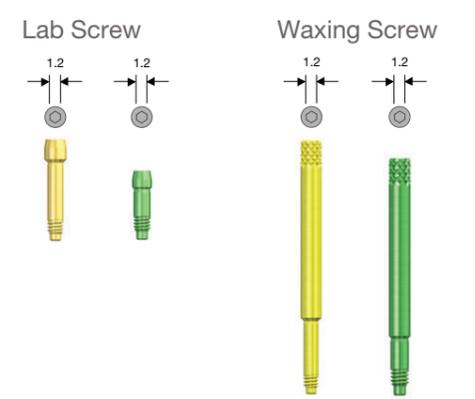

| Code | Mini | | Regular |
|------|--------------|---------|---------|
| | Lab Screw | GSABSML | GSABSSL |
| | Waxing Screw | GSABSMW | GSABSSW |

- Packing unit : Laboratory screw
- Lab Screw : Use for laboratory work instead of abutment screw.
- Waxing Screw : Use for making a screw hole of a transfer jig or wax-up part.


Fixture Lab Analog



| Code | Mini | Regular |
|------|----------|----------|
| | GSTLA350 | GSTLA400 |

- Oral fixtures are built on the working model
- Packing unit : Lab analog


Bite Index

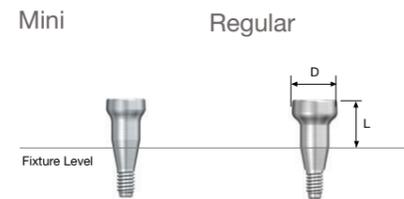


| L | D | Mini | Regular |
|------|---|------------|------------|
| | | ø 4.5 | ø 5.5 |
| 4.0 | | GSBIM4504S | GSBIS5504S |
| 6.0 | | GSBIM4506S | GSBIS5506S |
| 8.0 | | GSBIM4508S | GSBIS5508S |
| 10.0 | | GSBIM4510S | GSBIS5510S |
| 12.0 | | GSBIM4512S | GSBIS5512S |

- Use for taking a bite registration at Fixture level impression
- Use for taking a bite registration after final impression
- Use a 1.2 Hex driver
- Packing Unit: Bite Index 2ea

Fixture Pick-up Impression Coping

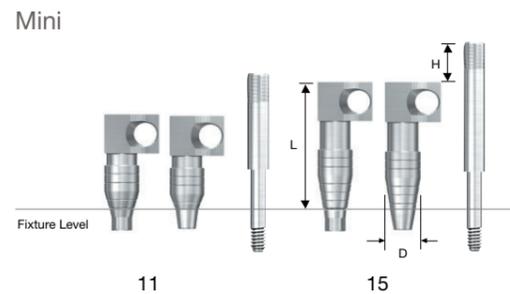


| L | Type | D | ø 4.0 | | | |
|---------------|---------|---|-------------|--|--|--|
| | | | | | | |
| 11 | Hex | | GSPIM4011 | | | |
| | Non-Hex | | GSPIM4011N | | | |
| Guide Pin (H) | 0 | - | GSPGPM100 | | | |
| | 5.0 | - | GSPGPM150* | | | |
| 15 | Hex | | GSPIM4015 | | | |
| | Non-Hex | | GSPIM4015N | | | |
| Guide Pin (H) | 0 | - | GSPGPM100L | | | |
| | 5.0 | - | GSPGPM150L* | | | |

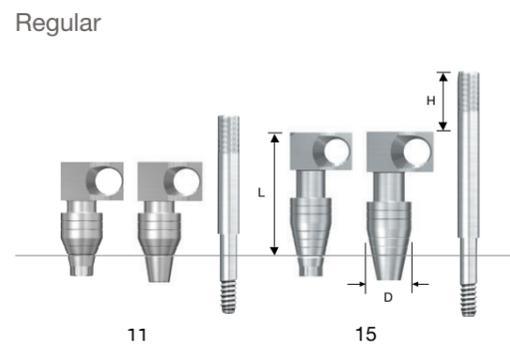


| L | Type | D | ø 4.0 | ø 5.0 | ø 6.0 | ø 7.0 |
|---------------|---------|---|-------------|------------|------------|------------|
| | | | | | | |
| 11 | Hex | | GSPIS4011 | GSPIS5011 | GSPIS6011 | GSPIS7011 |
| | Non-Hex | | GSPIS4011N | GSPIS5011N | GSPIS6011N | GSPIS7011N |
| Guide Pin (H) | 0 | - | GSPGPR100 | | | |
| | 5.0 | - | GSPGPR150* | | | |
| 15 | Hex | | GSPIS4015 | GSPIS5015 | GSPIS6015 | GSPIS7015 |
| | Non-Hex | | GSPIS4015N | GSPIS5015N | GSPIS6015N | GSPIS7015N |
| Guide Pin (H) | 0 | - | GSPGPR100L | | | |
| | 5.0 | - | GSPGPR150L* | | | |

- Pick-up type for taking an impression using a customized tray
- Impression coping designed with Hole-in-one ; no need for resin fixation
- Asymmetrical structure minimizing contact interference ()
- Long and short types enhance convenience.
- Packing unit : Impression Coping Body + Guide Pin


※ The connection of the fixture transfer impression coping can also be verified by aligning the notch (A) in the connecting part of the coping body with the upper part of the fixture or removing the gap at the 11° taper area.

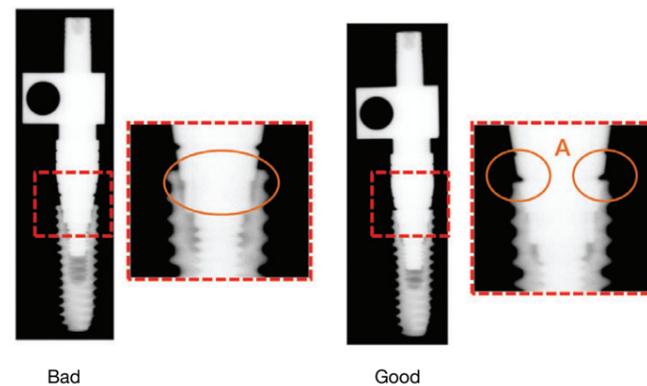

Fixture Transfer Impression Coping

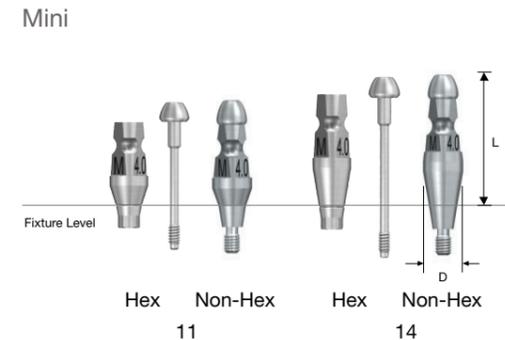


| L | Type | D | ø 4.0 | |
|----|---------|---|------------|--|
| | | | | |
| 11 | Hex | | GSTIM4011 | |
| | Non-Hex | | GSTIM4011N | |
| 14 | Hex | | GSTIM4014 | |
| | Non-Hex | | GSTIM4014N | |

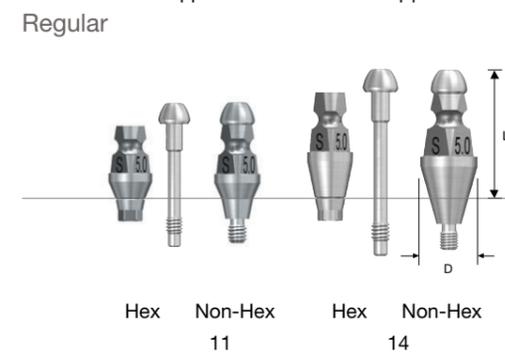


| L | Type | D | ø 4.0 | ø 5.0 | ø 6.0 |
|----|---------|---|------------|------------|------------|
| | | | | | |
| 11 | Hex | | GSTIS4011 | GSTIS5011 | GSTIS6011 |
| | Non-Hex | | GSTIS4011N | GSTIS5011N | GSTIS6011N |
| 14 | Hex | | GSTIS4014 | GSTIS5014 | GSTIS6014 |
| | Non-Hex | | GSTIS4014N | GSTIS5014N | GSTIS6014N |

- Transfer type for taking an impression using a ready-made tray
- Triangular arc () design improves markability following impression
- Long and short types enhance convenience
- The hex type is designed as a two-piece, and the non-hex type, as a one-piece
- Packing unit : Impression Coping Body + Guide Pin (Hex)
Impression Coping (Non-Hex)

Temporary Abutment

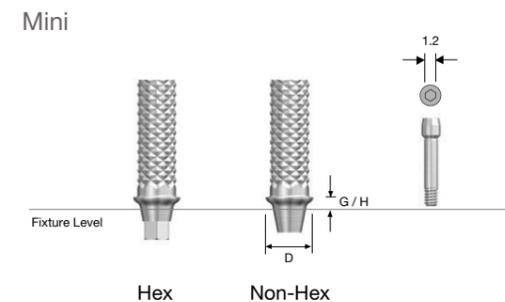

| G/H | Type | D | ø 4.0 | |
|----------|---------|---|-------------|--|
| | | | | |
| 1.0 | Hex | | GSTTA4010T | |
| | Non-Hex | | GSTTA4010TN | |
| 3.0 | Hex | | GSTTA4030T | |
| | Non-Hex | | GSTTA4030TN | |
| Ti Screw | | | GSABSMT | |

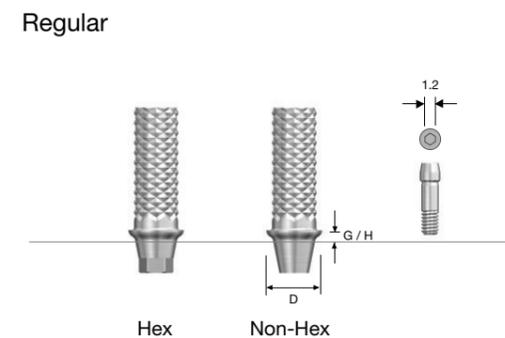


| G/H | Type | D | ø 4.5 | |
|----------|---------|---|-------------|--|
| | | | | |
| 1.0 | Hex | | GSTTA4510T | |
| | Non-Hex | | GSTTA4510TN | |
| 3.0 | Hex | | GSTTA4530T | |
| | Non-Hex | | GSTTA4530TN | |
| Ti Screw | | | GSABSST | |

- Use to make temporary prosthesis (material : Ti Gr-3)
- Easy to customize ; designed to minimize indication constraints
- Use a 1.2 hex driver
- Packing unit : Abutment + Ti screw
- Tightening torque : 20 Ncm (mini, regular)

Order code - Abutment + Ti screw : Product code + TH (ex : GSTTA4510TH)

Angled Abutment


Cement Retained Restoration

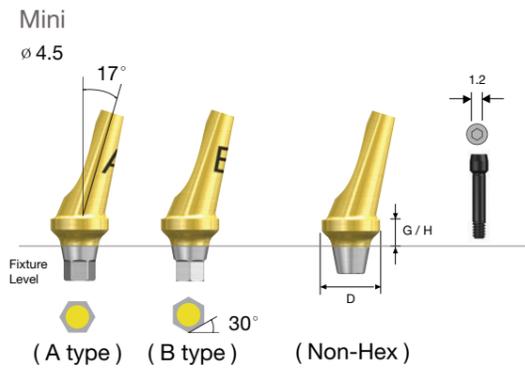

| G/H | Type | D | ø 4.5 |
|-----------------|-------------|---|------------|
| 2.0 | Hex(A Type) | | GSAA4520MA |
| | Hex(B Type) | | GSAA4520MB |
| | Non-Hex | | GSAA4520MN |
| 4.0 | Hex(A Type) | | GSAA4540MA |
| | Hex(B Type) | | GSAA4540MB |
| | Non-Hex | | GSAA4540MN |
| EbonyGold Screw | | | GSABSM |

Regular

ø 5.0

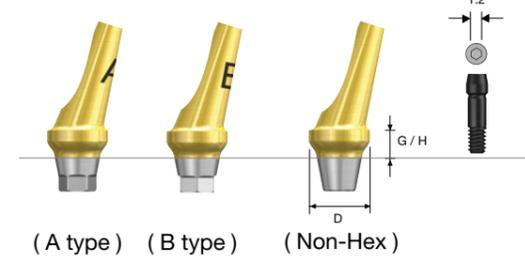


| G/H | Type | D | ø 5.0 | ø 6.0 |
|-----------------|-------------|---|-----------|-----------|
| 2.0 | Hex(A Type) | | GSAA5020A | GSAA6020A |
| | Hex(B Type) | | GSAA5020B | GSAA6020B |
| | Non-Hex | | GSAA5020N | GSAA6020N |
| 4.0 | Hex(A Type) | | GSAA5040A | GSAA6040A |
| | Hex(B Type) | | GSAA5040B | GSAA6040B |
| | Non-Hex | | GSAA5040N | GSAA6040N |
| EbonyGold Screw | | | GSABSS | |

- Used for the path adjustment of prosthesis in case of 17° axial angle
- 11° taper connection for excellent safety
- Gold color for aesthetic effect
- Functions as a double hex type (A and B hex types)
- The use of an abutment selector enables the selection of precise hex-type abutments
- Use a 1.2 hex driver
- Packing unit : Abutment + EbonyGold screw
- Tightening torque : 20 Ncm (mini), 30 Ncm (standard)

Order code
 - Abutment + EbonyGold screw : Product code + **WH** (ex : GSAA5020**AWH**)

ø 6.0

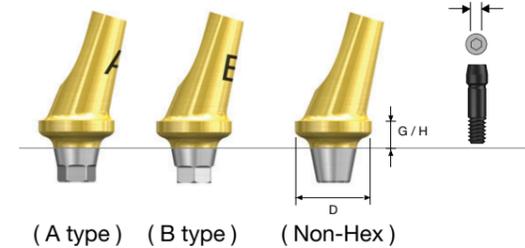

GS Angled Abutment Selector




| G / H | Type | D | Mini | | | Regular | | |
|-------|-------------|---|-------------|------------|------------|---------|-------|-------|
| | | | ø 4.5 | ø 5.0 | ø 6.0 | ø 4.5 | ø 5.0 | ø 6.0 |
| 2.0 | Hex(A Type) | | GSAAS4520MA | GSAAS5020A | GSAAS6020A | | | |
| | Hex(B Type) | | GSAAS4520MB | GSAAS5020B | GSAAS6020B | | | |
| 4.0 | Hex(A Type) | | GSAAS4540MA | GSAAS5040A | GSAAS6040A | | | |
| | Hex(B Type) | | GSAAS4540MB | GSAAS5040B | GSAAS6040B | | | |

- Use for the selection of specifications such as A- or B-type angled abutments, diameter, and G/H in the oral cavity or on a working model

ZioCera Abutment


Cement or Screw Retained Restoration

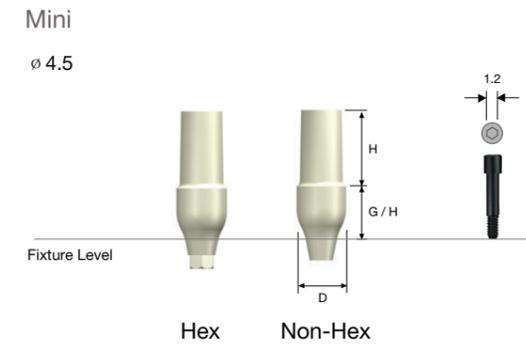

| D | | ø 4.5 | |
|-----------------|-----|---------|------------|
| H | G/H | Type | |
| 7.0 | 3.5 | Hex | GSZAM4535 |
| | 5.0 | Non-Hex | GSZAM4535N |
| | | Hex | GSZAM4550 |
| | | Non-Hex | GSZAM4550N |
| EbonyGold Screw | | | GSASM |


Regular

ø 4.5

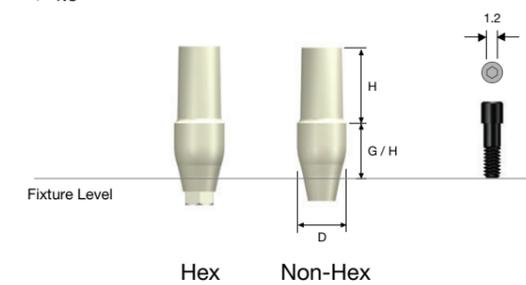


| D | | ø 4.5 | |
|-----------------|-----|---------|------------|
| H | G/H | Type | |
| 7.0 | 3.5 | Hex | GSZAS4535 |
| | 5.0 | Non-Hex | GSZAS4535N |
| | | Hex | GSZAS4550 |
| | | Non-Hex | GSZAS4550N |
| EbonyGold Screw | | | GSASR |

ø 5.5

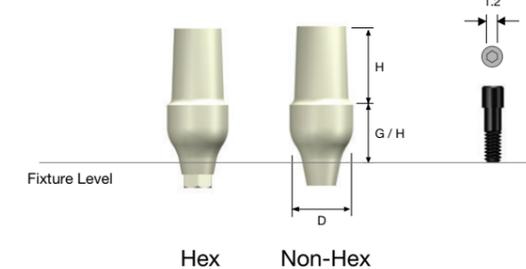

| D | | ø 5.5 | |
|-----------------|-----|---------|------------|
| H | G/H | Type | |
| 7.0 | 3.5 | Hex | GSZAS5535 |
| | 5.0 | Non-Hex | GSZAS5535N |
| | | Hex | GSZAS5550 |
| | | Non-Hex | GSZAS5550N |
| EbonyGold Screw | | | GSASR |

ø 6.5

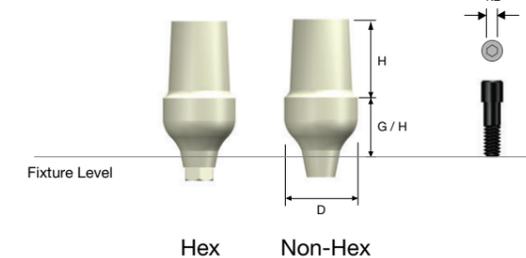


| D | | ø 6.5 | |
|-----------------|-----|---------|------------|
| H | G/H | Type | |
| 7.0 | 3.5 | Hex | GSZAS6535 |
| | 5.0 | Non-Hex | GSZAS6535N |
| | | Hex | GSZAS6550 |
| | | Non-Hex | GSZAS6550N |
| EbonyGold Screw | | | GSASR |

- Use for esthetic implant restorations
- Ivory Color for esthetic shade
- Applicable as a screw retained by direct build up
- Use a 1.2 Hex driver
- Packing Unit: Abutment + EbonyGold Screw
- Tightening torque: 20Ncm(mini), 30Ncm(regular)

Order code - Abutment + EbonyGold screw : Product Code + **WH**
 (ex : GSZAS5535**NWH**)

ZioCera Angled abutment
Cement or Screw Retained Restoration

Regular

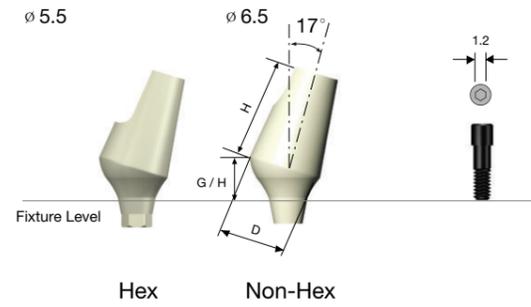

| D | | | ø 5.5 | |
|-----------------|-----|------|-------------|--------------|
| H | G/H | Type | Hex | Non-Hex |
| 9.0 | 3.0 | | GS17ZAS5530 | GS17ZAS5530N |
| | 4.0 | | - | - |
| EbonyGold Screw | | | GSASR | |


| D | | | ø 6.5 | |
|-----------------|-----|------|-------------|--------------|
| H | G/H | Type | Hex | Non-Hex |
| 9.0 | 3.0 | | - | - |
| | 4.0 | | GS17ZAS6540 | GS17ZAS6540N |
| EbonyGold Screw | | | GSASR | |

- Use for esthetic implant restorations which needed path modification
- Ivory Color for esthetic shade
- Applicable as a screw retained by direct build up
- Use a 1.2 Hex driver
- Packing Unit: Abutment + EbonyGold Screw
- Tightening torque: 20Ncm(mini), 30Ncm(regular)

Order code - Abutment + EbonyGold screw : Product Code + WH (ex : GS17ZAS5530NWH)


GoldCast Abutment
Screw or Cement Retained Restoration

Mini

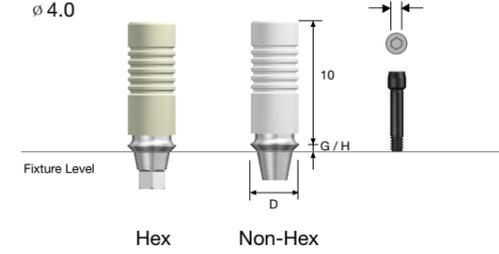

| G/H | Type | D | ø 4.0 |
|-----------------|---------|---|-----------|
| 1.0 | Hex | | GSGA4010S |
| | Non-Hex | | GSGA4010B |
| 3.0 | Hex | | GSGA4030S |
| | Non-Hex | | GSGA4030B |
| EbonyGold Screw | | | GSABSM |

Regular

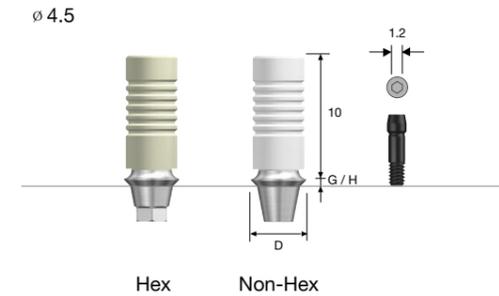

| G/H | Type | D | ø 4.5 |
|-----------------|---------|---|-----------|
| 1.0 | Hex | | GSGA4510S |
| | Non-Hex | | GSGA4510B |
| 3.0 | Hex | | GSGA4530S |
| | Non-Hex | | GSGA4530B |
| EbonyGold Screw | | | GSABSS |

- Use for cases with path and aesthetic and spatial constraints
- 11° taper connection for excellent safety
- After customization, be sure to use only dental gold alloy for casting to make the prosthesis
- Melting point range of abutments (Au, Pt, Pd Alloy) : 1400 - 1450° C (use of non-precious metal alloy for casting prohibited)
- Use a 1.2 hex driver
- Packing unit : Abutment + EbonyGold screw
- Tightening torque : 20 Ncm (mini), 30 Ncm (regular)


Order code

- Abutment + EbonyGold screw : Product code + WH (ex : GSGA4510SWH)

NP-CAST Abutment


Screw or Cement Retained Restoration

Mini

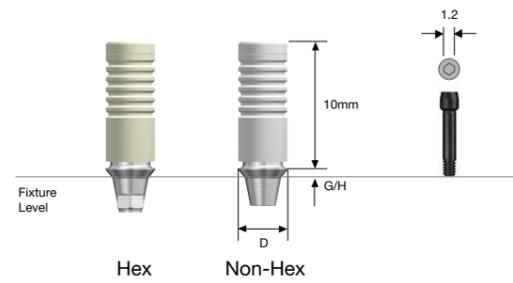

| G/H | Type | D | ∅ 4.0 |
|-----------------|---------|---|-----------|
| 1.0 | Hex | | GSNA4010S |
| | Non-Hex | | GSNA4010B |
| 3.0 | Hex | | GSNA4030S |
| | Non-Hex | | GSNA4030B |
| EbonyGold Screw | | | GSABSM |

Regular

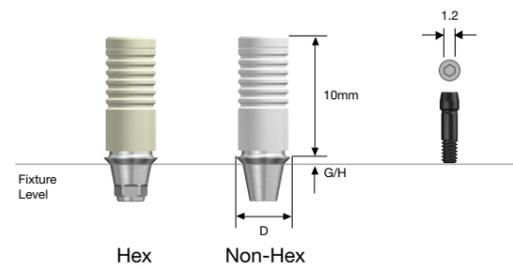

| G/H | Type | D | ∅ 4.5 |
|-----------------|---------|---|-----------|
| 1.0 | Hex | | GSNA4510S |
| | Non-Hex | | GSNA4510B |
| 3.0 | Hex | | GSNA4530S |
| | Non-Hex | | GSNA4530B |
| EbonyGold Screw | | | GSABSS |

• Packing unit : Abutment + EbonyGold screw


- Use for cases with path and aesthetic and spatial constraints
- After customization, be sure to use only dental non-precious metal alloy for casting to make the prosthesis
- Use the 1.2 hex driver
- Tightening torque : 20Ncm(Mini), 30Ncm(Regular)

Order code

- Abutment + EbonyGold screw : Product Code + **WH** (ex : GSNA4510S**WH**)

CustomFit Abutment

Cement Retained Restoration

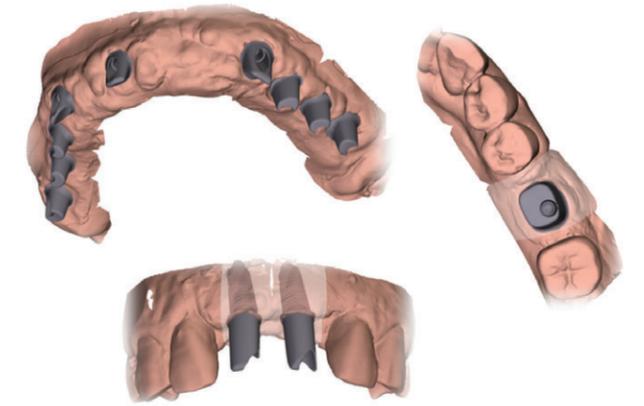

- CAD/CAM patient-specific abutment
- Use the 1.2 hex driver
- Tightening torque : 20Ncm(Mini), 30Ncm(Regular)

Recommended clinical cases


1. Case that the implant position and angle is deviated (Max. 30°)
2. Multiple case that requires consistent path and stable support
3. Case of anterior tooth part requiring esthetic design
4. Case of irregular or excessively deep gingiva

How to make an order

1. Fill the order sheet.
2. Inform the needed items to Osstem Implant CAD/CAM Center (free).
3. Working time : 5~7days


FreeForm ST Abutment
Cement Retained Restoration

Mini

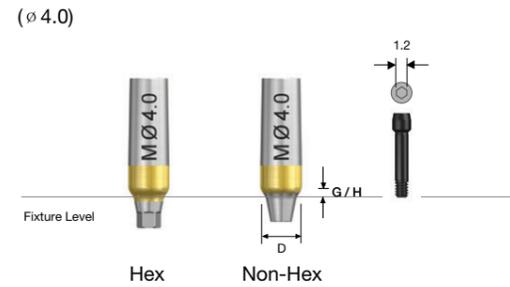

| G/H | Type | D | ∅ 4.0 |
|-----------------|---------|---|------------|
| 1.5 | Hex | | GSFAM4015 |
| | Non-Hex | | GSFAM4015N |
| 3.0 | Hex | | GSFAM4030 |
| | Non-Hex | | GSFAM4030N |
| EbonyGold Screw | | | GSABSM |

Regular

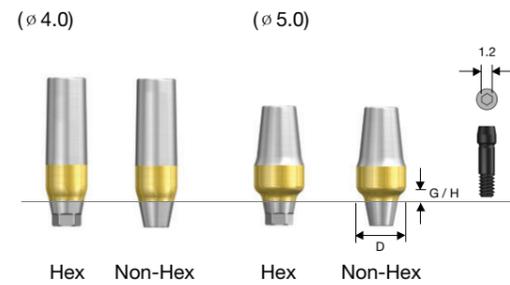


| G/H | Type | D | ∅ 4.0 | ∅ 5.0 | ∅ 6.0 | ∅ 7.0 |
|-----------------|---------|---|-----------|-----------|-----------|-----------|
| 1.5 | Hex | | GSFA4015 | GSFA5015 | GSFA6015 | GSFA7015 |
| | Non-Hex | | GSFA4015N | GSFA5015N | GSFA6015N | GSFA7015N |
| 3.0 | Hex | | GSFA4030 | GSFA5030 | GSFA6030 | GSFA7030 |
| | Non-Hex | | GSFA4030N | GSFA5030N | GSFA6030N | GSFA7030N |
| EbonyGold Screw | | | GSABSS | | | |

- Use for the path adjustment of abutments or customization of prosthetic margin
- 11° taper connection for excellent safety
- Gingival gold color for aesthetic effect
- Use a 1.2 hex driver
- Packing unit : Abutment + EbonyGold screw
- Tightening torque : 20 Ncm (mini), 30 Ncm (regular)

Order code

- Abutment + EbonyGold screw : Product code + **WH** (ex : GSFA5015**WH**)

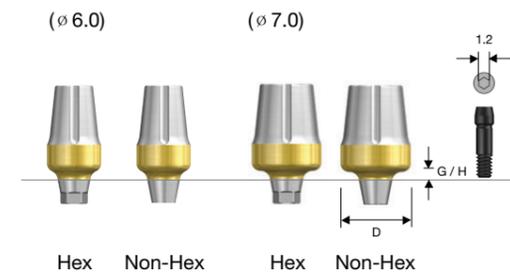


Convertible Abutment Components

Convertible Abutment


Screw & Cement Retained Restoration

Mini

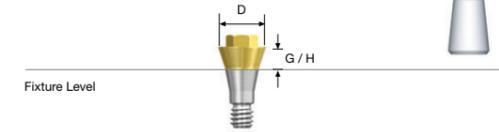

| G/H | D | ∅ 4.0 |
|-----|---|----------|
| 1.0 | | GSCA4010 |
| 2.0 | | GSCA4020 |
| 3.0 | | GSCA4030 |
| 4.0 | | GSCA4040 |

Regular

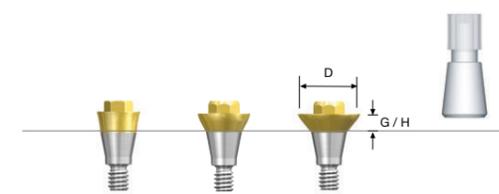


| G/H | D | ∅ 4.0 | ∅ 5.0 | ∅ 6.0 |
|-----|---|-----------|----------|----------|
| 1.0 | | GSCAS4010 | GSCA5010 | GSCA6010 |
| 2.0 | | GSCAS4020 | GSCA5020 | GSCA6020 |
| 3.0 | | GSCAS4030 | GSCA5030 | GSCA6030 |
| 4.0 | | GSCAS4040 | GSCA5040 | GSCA6040 |
| 5.0 | | - | GSCA5050 | GSCA6050 |

- Use for creating bridge case prosthesis with dislocated path
- Designed to make the prosthesis onto a cylinder following abutment connection in the oral cavity
- ∅ 4.0 : Use an O-ring abutment driver
∅ 4.8, ∅ 6.0 : Use an Octa abutment driver
- Packing : Abutment + Carrier
- Tightening torque : 30 Ncm

Order code - Abutment + Carrier : Product Code + **P** (ex : GSCA5030**P**)

Convertible Combination Cylinder

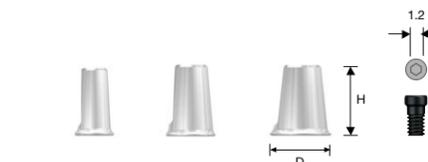


| H | D | Mini | Regular | | |
|-----------------|---|---------------------|------------------|------------------|-------|
| | | ∅ 4.0 | ∅ 4.0 | ∅ 5.0 | ∅ 6.0 |
| 7.0 | | GSCC4070T(Hex) | GSCC5070T (Octa) | GSCC6070T (Octa) | |
| | | GSCC4070TN(Non-Hex) | | | |
| EbonyGold Screw | | GSFSM | GSFSR | | |

- Use for making combination-retained prosthesis using convertible abutments.
- Use a 1.2 hex driver
- Packing unit : Cylinder + EbonyGold screw
- Tightening torque : 20 Ncm

Order code

- Cylinder + EbonyGold screw : Product code + **WH** (ex : GSCC5070T**WH**)

Convertible Angled Cylinder

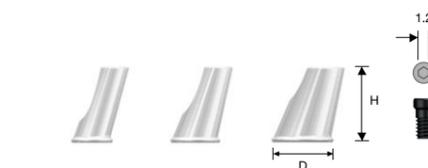


| H | D | Mini | Regular | | |
|-----------------|---|---------------------|------------------|------------------|-------|
| | | ∅ 4.0 | ∅ 4.0 | ∅ 5.0 | ∅ 6.0 |
| 8.0 | | GSAC4080T(Hex) | GSAC5080T (Octa) | GSAC6080T (Octa) | |
| | | GSAC4080TN(Non-Hex) | | | |
| EbonyGold Screw | | GSFSM | GSFSR | | |

- Use for making combination-retained prosthesis using convertible abutments
- Used for the path adjustment of prosthesis given 17° axial angle
- Use a 1.2 hex driver
- Packing unit : Cylinder + EbonyGold screw
- Tightening torque : 20 Ncm

Order code

- Cylinder + EbonyGold screw : Product Code + **WH** (ex : GSAC5080T**WH**)

Convertible GoldCast Cylinder

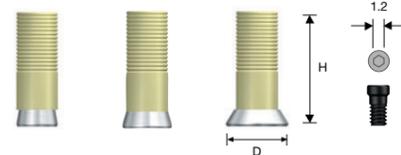


| | | Mini | | Regular | |
|-----------------|---|-------------------|-------|----------------|----------------|
| H | D | ø 4.0 | ø 4.0 | ø 5.0 | ø 6.0 |
| 12 | | GSGC400(Hex) | | GSGC500 (Octa) | GSGC600 (Octa) |
| | | GSGC400N(Non-Hex) | | | |
| EbonyGold Screw | | GSFSM | | GSFSR | |

- Use for making screw-retained prosthesis using convertible abutments
- After customization, be sure to use only dental gold alloy for casting to make the prosthesis
- Melting point range of cylinder (Au, Pt, Pd Alloy) : 1400 - 1450° C (use of non-precious metal alloy for casting prohibited)
- Use a 1.2 hex driver
- Packing unit : Cylinder + EbonyGold screw
- Tightening torque : 20 Ncm

Order code - Cylinder + EbonyGold screw : Product Code + **WH**
(ex: GSGC500**WH**)

Convertible Temporary Cylinder

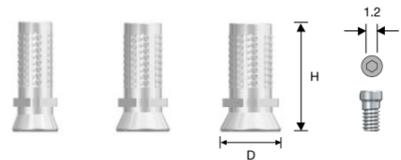


| | | Mini | | Regular | |
|----------|---|---------------------|-------|------------------|------------------|
| H | D | ø 4.0 | ø 4.0 | ø 5.0 | ø 6.0 |
| 10 | | GSCTC400T(Hex) | | GSCTC500T (Octa) | GSCTC600T (Octa) |
| | | GSCTC400TN(Non-Hex) | | | |
| Ti Screw | | GSFSMT | | GSFSRT | |

- Use to make temporary prosthesis (material: Ti Gr-3)
- Easy to customize ; designed to minimize indication constraints
- Use a 1.2 hex driver
- Packing unit : Cylinder + EbonyGold screw
- Tightening torque : 20 Ncm

Order code - Cylinder + Ti screw : Product Code + **TH** (ex: GSCTC500**TTH**)

Convertible Plastic Cylinder

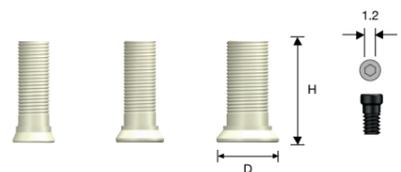

| | | Mini | | Regular | |
|-----------------|---|--------------------|-------|-----------------|-----------------|
| H | D | ø 4.0 | ø 4.0 | ø 5.0 | ø 6.0 |
| 12 | | GSCPL400(Hex) | | GSCPL500 (Octa) | GSCPL600 (Octa) |
| | | GSCPL400N(Non-Hex) | | | |
| EbonyGold Screw | | GSFSM | | GSFSR | |

- Use for making screw-retained prosthesis using convertible abutments
- After customization, casting should be performed with dental alloy (gold, non-precious metal) to make the prosthesis
- The precision of the connection part is lower compared to gold cylinders
- Use a 1.2 hex driver
- Packing unit : Cylinder + EbonyGold screw
- Tightening torque : 20 Ncm

Order code - Cylinder + EbonyGold screw : Product Code + **WH**
(ex: GSCPL500**WH**)

Convertible Pick-up Impression Coping



| | | Mini | | Regular | |
|---------------|---|---------------|-------|-----------------|-----------------|
| D | | ø 4.0 | ø 4.0 | ø 5.0 | ø 6.0 |
| Code | | GSPIC400(Hex) | | GSPIC500 (Octa) | GSPIC600 (Octa) |
| Guide Pin (H) | 0 | GSCGP400S | | GSCGP500S | |
| | 5 | GSCGP400L* | | GSCGP500L | |

- Pick-up type for taking an impression using a customized tray
- Impression coping designed with Hole-in-one ; no need for resin fixation
- Asymmetrical structure minimizing contact interference ()
- Packing unit : Impression coping body + Guide Pin


Convertible Transfer Impression Coping



| | | Mini | | Regular | |
|------|--|---------------|-------|-----------------|-----------------|
| D | | ø 4.0 | ø 4.0 | ø 5.0 | ø 6.0 |
| Code | | GSTIC400(Hex) | | GSTIC500 (Octa) | GSTIC600 (Octa) |

- Transfer type for taking an impression using a ready-made tray
- Triangular arc () design improves markability following impression
- Packing unit : Impression Coping body + Guide Pin

Convertible Protect Cap

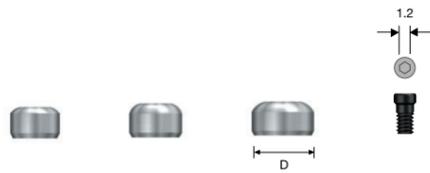

| | Mini | Regular | |
|-----------------|---------------|---------|---------------------|
| D | ø 4.0 | ø 4.0 | ø 5.0 |
| Code | GSCHC400(Hex) | | GSCHC500 (Non-Octa) |
| EbonyGold Screw | GSFSM | | GSFSR |

- Use for the protection of Convertible abutments in the oral cavity and to minimize the patient's discomfort
- Use a 1.2 hex driver
- Packing unit : Protect Cap + EbonyGold screw
- Tightening torque : 20Ncm

Order code

- Protect Cap + EbonyGold screw : Product Code + **WH** (ex: GSCHC500**WH**)

Convertible Lab Analog



| | Mini | Regular | |
|------|----------|---------|----------|
| D | ø 4.0 | ø 4.0 | ø 5.0 |
| Code | GSCLA400 | | GSCLA500 |
| | | | GSCLA600 |

- Make aesthetic oral abutments on the working model
- Packing unit : Lab analog

Convertible Polishing Protector




| | Mini | Regular | |
|------|---------------|----------------|----------------|
| D | ø 4.0 | ø 5.0 | ø 6.0 |
| Code | GSCPC400(Hex) | GSCPC500(Octa) | GSCPC600(Octa) |

- For polishing upon prosthetic casting, use to avoid damaging the cylinder joint
- Packing unit : Polishing protector

Stud Abutment Components


Stud Abutment Overdenture Restoration

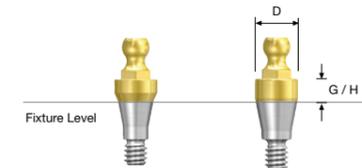

| | Mini | Regular |
|---------|-----------|----------|
| G/H \ D | ø 3.5 | ø 3.5 |
| 1.0 | GSSAM3510 | GSSA3510 |
| 2.0 | GSSAM3520 | GSSA3520 |
| 3.0 | GSSAM3530 | GSSA3530 |
| 4.0 | GSSAM3540 | GSSA3540 |
| 5.0 | GSSAM3550 | GSSA3550 |
| 6.0 | GSSAM3560 | GSSA3560 |

- Packing unit : Only abutment


Stud Abutment Set (Dalbo Set) Overdenture Restoration

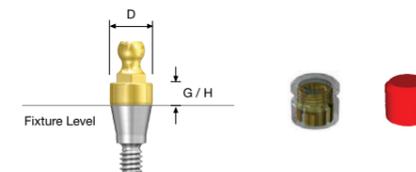

| | Mini | Regular |
|---------|------------|-----------|
| G/H \ D | ø 3.5 | ø 3.5 |
| 1.0 | GSSAM3510D | GSSA3510D |
| 2.0 | GSSAM3520D | GSSA3520D |
| 3.0 | GSSAM3530D | GSSA3530D |
| 4.0 | GSSAM3540D | GSSA3540D |
| 5.0 | GSSAM3550D | GSSA3550D |
| 6.0 | GSSAM3560D | GSSA3560D |

- Use for making stud-type overdenture
- Superior stability of retention force vs. O-ring
- Dalbo plus attachment components
Housing(Ti) + internal lamella(Gold alloy)
Duplicate aid (plastic)
- Recover the retention force through internal lamella rotation (clockwise) using a special-purpose driver
- Maximum path compensation of 20°
- Use an O-ring abutment driver
- Packing unit : Abutment + Dalbo plus attachments
- Tightening torque: 30 Ncm

※ Due to a mix of specifications(Mini/Regular) will occur wrong connection.
Always verify the exactness of the connection by taking an x-ray after the final connection of the abutment.

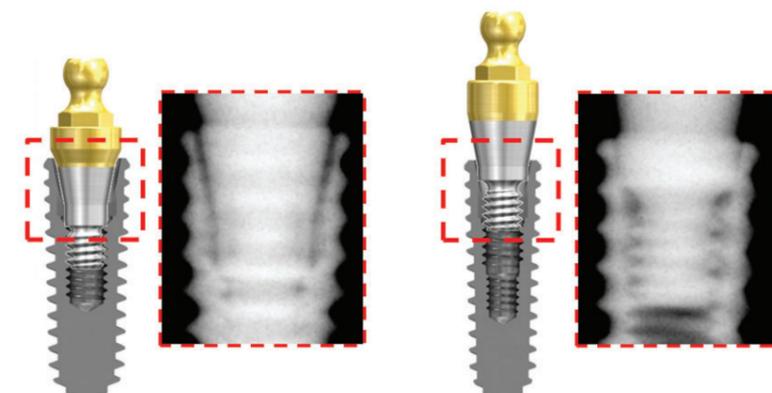

< Abutment : Mini / Fixture : Regular >

< Abutment : Regular / Fixture : Mini >

O-ring Retainer Cap Set

| | |
|------|-------|
| Code | RCS01 |
|------|-------|

- Packing unit : Retainer cap + O-ring



O-ring Retainer Set

| | |
|------|------|
| Code | RS01 |
|------|------|

- More advantageous for smaller occlusal gap compared to a retainer cap
- Packing unit : Retainer + O-ring



O-ring Set

| | |
|------|---------|
| Code | OAON01S |
|------|---------|

- Packing unit : O-ring 5 piece



O-ring Lab Analog

| | |
|------|-----|
| Code | OAL |
|------|-----|


- Make oral O-ring abutments on the working model
- Packing unit : Lab analog




LOCATOR® Components

LOCATOR® Abutment Overdenture Restoration

Mini



Regular



| | | Mini | Regular |
|-----|---|------------|------------|
| G/H | D | ø 3.7 | |
| 1.0 | | HGLCA3510M | HGLCA4010S |
| 2.0 | | HGLCA3520M | HGLCA4020S |
| 3.0 | | HGLCA3530M | HGLCA4030S |
| 4.0 | | HGLCA3540M | HGLCA4040S |
| 5.0 | | HGLCA3550M | HGLCA4050S |

- Packing unit : Locator abutment
- Stable dual retention & optimal holding capabilities against various retention forces (6N, 12N, 22N)
- Excellent durability
- Possible denture restorations even at small vertical dimension
- Accommodate up to 40° divergence between two implants
- Retention males can be easily placed & removed with core tool
- Tightening torque : 30Ncm
- Can be used in GS system & HG system

LOCATOR® Male Processing Kit



| Code | LMPS |
|------|------|
|------|------|

- Packing Unit : Locator Male Processing Kit (2 Set)
- Consist of
 - Block out Spacer/Denture Cap connected Black Processing Male
 - Replacement Male Blue/Pink/Clear
- Male Change by Locator Core Tool

LOCATOR® Replacement Male



| Code | LRM06S |
|------|--------|
|------|--------|

- Packing Unit : Blue Replacement Male (4ea)
- retention Force : about 6N
- 0° ~20° divergence (between two implants)

| Code | LRM12S |
|------|--------|
|------|--------|

- Packing Unit : Pink Replacement Male (4ea)
- retention Force : about 12N
- 0° ~20° divergence (between two implants)

| Code | LRM22S |
|------|--------|
|------|--------|

- Packing Unit : clear Replacement Male (4ea)
- retention Force : about 22N
- 0° ~20° divergence (between two implants)

LOCATOR® Extended Replacement Male



| Code | LEM06S |
|------|--------|
|------|--------|

- Packing Unit : Red Extended Replacement Male (4ea)
- retention Force : about 6N
- 20° ~40° divergence (between two implants)

| Code | LEM12S |
|------|--------|
|------|--------|

- Packing Unit : Green Extended Replacement Male (4ea)
- retention Force : about 12N
- 20° ~40° divergence (between two implants)

LOCATOR® Black Processing Male



| Code | LBPS |
|------|------|
|------|------|

- Packing Unit : black processing Male (4ea)
- for lab. process

LOCATOR® Block out spacers



| Code | LBSS |
|------|------|
|------|------|

- Packing Unit : Locator Block out spacers (20ea)
- For Space Sealing between Locator Abutment & Denture Cap

LOCATOR® Impression Coping



| Code | LICS |
|------|------|
|------|------|

- Packing Unit : Locator Impression Coping (4ea)
- For Abutment level impression

LOCATOR® lab Analog



| Code | LAL40S |
|------|--------|
| | LAL50S |

- Packing Unit : Locator lab Analog (4ea)

LOCATOR® Core Tool

| Code | LCCT |
|------|------|
|------|------|

- Packing Unit : Locator Core Tool
- foe handling of locator system



LOCATOR® Torque Driver

| Type | Short | Long |
|------|-------|-------|
| Code | TWLDS | TWLDL |

- Packing Unit : Locator Torque Driver
- For tightening of Locator Abutment
- Select the Short/Long length



OSSTEM[®]
IMPLANT

